SIEMENS

*Artis zee*
*VC13*

[redacted] AX

# DICOM Conformance Statement

Rev. 08 20-Oct-2009

© Siemens AG, Healthcare Sector 2009
All rights reserved

Siemens AG, Healthcare Sector,
Henkestr. 127, D-91050 Erlangen, Germany
Siemensstr. 1, D-91301 Forchheim, Germany

Headquarters: Berlin and Munich
Siemens AG, Wittelsbacher Platz 2, D-80333 Munich, Germany

Printed in the Federal Republic of Germany

*syngo* is a registered trademark of Siemens AG.

# Table of Contents

*1 Introduction ..... 10*
**1.1 Overview ..... 10**
**1.2 Scope and Field ..... 10**
**1.3 Audience ..... 10**
**1.4 Remarks ..... 10**
**1.5 Definitions, Terms and Abbreviations ..... 11**
**1.6 References ..... 11**
**1.7 Structure ..... 11**
*2 Implementation Model Verification ..... 13*
**2.1 Application Data Flow Diagram ..... 13**
**2.2 Functional Definitions of Applications ..... 13**
**2.3 Sequencing of Real-World Activities ..... 13**
*3 Application Entity Specification Verification ..... 14*
**3.1 Verification AE Specification ..... 14**
3.1.1 Association Establishment Policies ..... 14
3.1.1.1 General ..... 14
3.1.1.2 Number of Associations ..... 14
3.1.1.3 Asynchronous Nature ..... 14
3.1.1.4 Implementation Identifying Information ..... 14
3.1.2 Association Initiation Policy ..... 14
3.1.2.1 Associated Real-World Activity - Verification ..... 14
3.1.3 Association Acceptance Policy ..... 15
*4 Implementation Model Storage ..... 16*
**4.1 Application Data Flow Diagram ..... 16**
**4.2 Functional Definitions of Application Entities ..... 16**
**4.3 Sequencing of Real-World Activities ..... 16**
*5 Application Entity Specification Storage ..... 17*
**5.1 Storage AEs Specification ..... 17**
5.1.1 Association Establishment Policies ..... 18
5.1.1.1 General ..... 18
5.1.1.2 Number of Associations ..... 18
5.1.1.3 Asynchronous Nature ..... 18
5.1.1.4 Implementation Identifying Information ..... 18
5.1.2 Association Initiation Policy ..... 18
5.1.2.1 Associated Real-World Activity - Send ..... 18
5.1.3 Association Acceptance Policy ..... 22
5.1.3.1 Associated Real-World Activity - Receive ..... 22
*6 Implementation Model Storage Commitment ..... 27*

**6.1 Application Data Flow Diagram ..... 27**
**6.2 Functional Definitions of Application Entities ..... 27**
**6.3 Sequencing of real World Activities ..... 27**
***7 AE Specification Storage Commitment ..... 28***
**7.1 Storage Commitment AE Specification ..... 28**
7.1.1 Association Establishment Policies ..... 28
7.1.1.1 General ..... 28
7.1.1.2 Number of Associations ..... 28
7.1.1.3 Asynchronous Nature ..... 28
7.1.1.4 Implementation Identifying Information ..... 28
7.1.2 Association Initiation Policy ..... 28
7.1.2.1 Real World Activity – Storage Commitment ..... 29
***8 Implementation Model Query / Retrieve ..... 31***
**8.1 Application Data Flow Diagram ..... 31**
**8.2 Functional Definitions of Application Entities ..... 32**
**8.3 Sequencing of Real-World Activities ..... 32**
***9 Application Entity Specification Query/Retrieve ..... 33***
**9.1 Query/Retrieve Service AEs Specification ..... 33**
9.1.1 Association Establishment Policies ..... 34
9.1.1.1 General ..... 34
9.1.1.2 Number of Associations ..... 34
9.1.1.3 Asynchronous Nature ..... 34
9.1.1.4 Implementation Identifying Information ..... 34
9.1.2 Association Initiation Policy ..... 34
9.1.2.1 Real World Activity - Find SCU ..... 34
9.1.2.2 Real-World Activity – Move SCU ..... 38
9.1.3 Association Acceptance Policy ..... 39
9.1.3.1 Real-World Activity - Find SCP ..... 39
9.1.3.2 Real-World Activity - Get SCP ..... 45
9.1.3.3 Real-World Activity - Move SCP ..... 46
***10 Implementation Model Print ..... 48***
**10.1 Application Data Flow Diagram ..... 48**
**10.2 Functional Definition of Application Entities ..... 48**
**10.3 Sequencing of Real-World Activities ..... 48**
***11 Application Entity Specification Print ..... 49***
**11.1 Print Management AE Specification ..... 49**
11.1.1 Association Establishment Policies ..... 49
11.1.1.1 General ..... 49
11.1.1.2 Number of Associations ..... 49
11.1.1.3 Asynchronous Nature ..... 49
11.1.1.4 Implementation Identifying Information ..... 50
11.1.2 Association Initiation Policy ..... 50
11.1.2.1 Associated Real-World Activity ..... 50
11.1.3 Association Acceptance Policy ..... 55
***12 Implementation Model Worklist ..... 56***
**12.1 Application Data Flow Diagram ..... 56**

**12.2 Functional Definitions of Application Entities ..... 56**
**12.3 Sequencing of Real-World Activities ..... 56**
***13 Application Entity Specification Worklist ..... 57***
**13.1 Modality Worklist Service AE Specification ..... 57**
13.1.1 Association Establishment Policies ..... 57
13.1.1.1 General ..... 57
13.1.1.2 Number of Associations ..... 57
13.1.1.3 Asynchronous Nature ..... 57
13.1.1.4 Implementation Identifying Information ..... 57
13.1.2 Association Initiation Policy ..... 58
13.1.2.1 Real-World Activity ..... 58
***14 Implementation Model MPPS ..... 65***
**14.1 Application Data Flow Diagram ..... 65**
**14.2 Functional Definitions of Application Entities ..... 65**
**14.3 Sequencing of real World Activities ..... 65**
***15 AE Specification MPPS ..... 66***
**15.1 Modality Performed Procedure Step AE Specification ..... 66**
15.1.1 Association Establishment Policies ..... 66
15.1.1.1 General ..... 66
15.1.1.2 Number of Associations ..... 66
15.1.1.3 Asynchronous Nature ..... 66
15.1.1.4 Implementation Identifying Information ..... 66
15.1.2 Association Initiation Policy ..... 66
15.1.2.1 Real World Activity ..... 67
***16 Communication Profiles ..... 73***
**16.1 Supported Communication Stacks ..... 73**
16.1.1 TCP/IP Stack ..... 73
16.1.1.1 API ..... 73
16.1.1.2 Physical Media Support ..... 73
***17 Extensions / Specializations / Privatizations ..... 74***
17.1.1 Standard Extended / Specialized / Private SOPs ..... 74
17.1.2 Private Transfer Syntaxes ..... 74
***18 Configuration ..... 75***
**18.1 AE Title/Presentation Address Mapping ..... 75**
18.1.1 DICOM Verification ..... 75
18.1.2 DICOM AE Titles ..... 75
18.1.2.1 DICOM Storage AE Title ..... 75
18.1.2.2 DICOM Query/Retrieve AE Title ..... 75
18.1.2.3 DICOM Print AE Title ..... 75
18.1.2.4 DICOM Modality Worklist AE Title ..... 75
**18.2 Configurable Parameters ..... 76**
18.2.1 Storage, Storage Commitment and Query/Retrieve ..... 76
18.2.2 Print ..... 76
18.2.3 Modality Worklist ..... 77
**18.3 Default Parameters ..... 77**
***19 Support of Extended Character Sets ..... 79***
***20 Artis zee VC13 Offline Media Application Profile ..... 80***

**20.1 Class and Profile Identification ..... 80**

**20.2 Clinical Context ..... 80**
20.2.1 Roles and Service Class Options ..... 80
20.2.1.1 File Set Creator ..... 81
20.2.1.2 File Set Reader ..... 81
20.2.1.3 File Set Updater ..... 81

**20.3 PRI-XAMAS Profiles ..... 82**
20.3.1 SOP Classes and Transfer Syntaxes ..... 82
20.3.2 Physical Media and Formats ..... 82
20.3.3 Directory Information in DICOMDIR ..... 82
20.3.3.1 Basic Directory IOD Specialization Option ..... 83
20.3.3.2 Additional Keys ..... 83
20.3.3.3 Private Directory Record Keys ..... 84
20.3.3.4 Icon Images ..... 84
20.3.4 Other Parameters ..... 84
20.3.4.1 Multi-Frame JPEG Format ..... 85
20.3.4.2 Attribute Value Precedence ..... 85

***21 Application Profile Conformance Statement ..... 86***

**21.1 Introduction ..... 86**
21.1.1 Purpose ..... 86
21.1.2 Scope ..... 86
21.1.3 Definitions, Abbreviations ..... 86
21.1.3.1 Definitions ..... 86
21.1.4 Abbreviations ..... 86
21.1.5 References ..... 87
21.1.6 Remarks ..... 87

**21.2 Implementation Model ..... 88**
21.2.1 Application Data Flow Diagram ..... 88
21.2.2 Functional Definitions of AEs ..... 88
21.2.3 Sequencing of Real-World Activities ..... 88
21.2.4 File Meta Information Options ..... 89

**21.3 AE Specifications ..... 89**
21.3.1 DICOM Archive Specification ..... 89
21.3.1.1 File Meta Information for the Application Entity ..... 89
21.3.1.2 Real-World Activities for this Application Entity ..... 89

**21.4 Augmented and Private Profiles ..... 91**
21.4.1 Augmented Application Profiles ..... 91
21.4.2 Private Application Profiles ..... 91
21.4.2.1 PRI-XAMAS-CD ..... 91

**21.5 Extensions, Specialization and Privatization of SOP Classes and Transfer Syntaxes ..... 91**
21.5.1 SOP Specific Conformance Statement for Basic Directory ..... 91
21.5.1.1 Extension, Specialization for SIEMENS Non-Image Objects ..... 91

**21.6 Configuration ..... 92**
21.6.1 AE Title Mapping ..... 92
21.6.1.1 DICOM Media Storage AE Title ..... 92

**21.7 Support of Extended Character Sets ..... 92**

***Annex A: Additional Information ..... 93***

**A.1 SIEMENS Private Non-Image IOD ..... 93**

**A.2 Siemens Standard Extended Modules ..... 97**

**A.3 Registry of private DICOM Data Elements ..... 107**
**A.4 Extended XA IOD ..... 111**
**A.5 Private Non-Image IOD ..... 115**
**A.6 Quant Report Images ..... 116**
**A.7 CT/MR Image Converted to XA IOD ..... 119**
**A.8 Sorting Order Artis zee VC13 ..... 124**
**A.9 Supported Matrix Sizes of Artis zee VC13 ..... 132**
**A.10 DICOM Print SCU – detailed status displays ..... 133**

# Table of Tables

Table 1 List of products applicable to this Conformance Statement 10
Table 2 Implementation Identifying Information 14
Table 3 Proposed Presentation Contexts 15
Table 4 Supported SOP Classes as an SCU 17
Table 5 Supported private SOP Classes as an SCU 17
Table 6 Supported SOP Classes as an SCP 17
Table 7 Supported private SOP Classes as an SCP 17
Table 8 Implementation Identifying Information 18
Table 9 Proposed Presentation Context – Send Images 19
Table 10 Resized images attributes 21
Table 11 Proposed Presentation Context – Receiving Images 23
Table 12 Attributes with applied defaults 24
Table 13 Storage Commitment SOP Class supported 28
Table 14 Implementation Identifying Information 28
Table 15 Proposed Presentation contents – request Storage Commitment 29
Table 16 Accepted Presentation contents – request Storage Commitment 30
Table 17 Supported SOP Classes as SCU 33
Table 18 Supported SOP Classes as SCP 33
Table 19 Implementation Identifying Information 34
Table 20 Proposed Presentation Contexts - Find SCU 35
Table 21 Search keys for Query models - Find SCU 37
Table 22 C-FIND response status 37
Table 23 Proposed Presentation Contexts - Move SCU “Import” 38
Table 24 Status Codes - Move SCU “Import” 39
Table 25 Accepted Presentation Contexts - Find SCP 40
Table 26 Supported Query attributes sorted by Query Level – Patient Root Information Model 42
Table 27 Supported Query attributes sorted by Query Level – Study Root Information Model 44
Table 28 Supported Query attributes sorted by Query Level – Patient/Study only Information Model 44
Table 29 Status Codes 44
Table 30 Accepted Presentation Contexts - Get SCP 45
Table 31 Status Codes 46
Table 32 Accepted Presentation Contexts - Move SCP 46
Table 33 Status Codes 47
Table 34 Basic Grayscale Print Management Meta SOP Class 49
Table 35 Implementation Identifying Information 50
Table 36 Proposed Presentation Contexts 51
Table 37 Used Basic Film Session N-CREATE-RQ attributes 52
Table 38 Attributes of N-DELETE-RQ on Basic Film Session SOP Class 52
Table 39 Basic Film Session SOP Status 52
Table 40 Used Film Box N-CREATE-RQ attributes 53
Table 41 Attributes of N-DELETE-RQ on Basic Film Session SOP Class 53
Table 42 Basic Film Session SOP Status 53
Table 43 Mandatory Basic Grayscale Image Box N-SET attributes 54
Table 44 Basic Grayscale Image Box SOP Status 54
Table 45 Used Printer N-EVENT report attributes 54
Table 46 Mandatory Printer N-GET-RSP, N-EVENT-RQ attributes 54
Table 47 Used Print Job N-EVENT-REPORT attributes 55
Table 48 SOP Classes as a SCU 57
Table 49 Implementation Identifying Information 57
Table 50 Proposed Presentation Contexts 58
Table 51 Supported Broad Worklist Query Search Key Attributes 59
Table 52 Basic Worklist C-FIND-RSP Return Key Attributes 62
Table 53 Patient based "narrow query" Search Key Attributes 63
Table 54 C-FIND-RSP Status 64
Table 55 SOP Classes as an SCU 66
Table 56 Implementation Identifying Information 66

© Siemens AG, Healthcare Sector, 2009 

*Table 57 Proposed Presentation Contexts - MPPS* 67
*Table 58 Performed Procedure Step N-CREATE Attributes* 69
*Table 59 MPPS N-CREATE Response Status* 69
*Table 60 Performed Procedure Step N-SET Attributes* 71
*Table 61 MPPS N-SET Response Status* 72
*Table 62 Ready-processed configuration* 76
*Table 63 PRI-XAMAS Universal Angio/Radio Class Profile* 80
*Table 64 PRI-XAMAS SOP Classes and Transfer Syntaxes* 82
*Table 65 Abbreviations for Transfer Syntaxes* 82
*Table 66 PRI-XAMAS Additional DICOMDIR Keys* 84
*Table 67 PRI-XAMAS Additional PRIVATE Record Keys* 84
*Table 68 File Meta Information Options* 89
*Table 69 Application profiles, Activities, and Roles for DICOM Archive* 89
*Table 70 STD-GEN-CD Supported SOP Classes for FSR Role* 90
*Table 71 Extension, Specialization for SIEMENS Non-Image Objects* 91
*Table 72 SIEMENS Private Non-Image IOD* 93
*Table 73 CSA Non-Image IOD Modules* 95
*Table 74 CSA Non-Image Attributes* 96
*Table 75 CSA Image IOD Modules* 97
*Table 76 MEDCOM Header Modules* 99
*Table 77 MEDCOM History Information* 99
*Table 78 MEDCOM OOG Module* 99
*Table 79 Edge Enhancement Module* 100
*Table 80 Angio Viewing Module* 101
*Table 81 Angio Acquisition Data Module* 103
*Table 82 Angio Quantification Module* 104
*Table 83 Original Image Info Module* 105
*Table 84 Image Type Extensions* 106
*Table 85 Private Elements in Group 0019* 107
*Table 86 Private Elements in Group 0021* 108
*Table 87 Private Elements in Group 0023* 108
*Table 88 Private Elements in Group 0025* 109
*Table 89 Private Elements in Group 0029 and 7FE1* 110
*Table 90 Private Elements in Group 2121* 110
*Table 91 Overview of supplied attributes- X-Ray-Angiographic images (Original, Derived)* 114
*Table 92 Data Dictionary of private IOD Definition – Exam Protocol* 115
*Table 93 Overview of supplied attributes- X-Ray-Angiographic image (Quant Report Image)* 118
*Table 94 Overview of supplied attributes- XA image (Derived) from CT image* 121
*Table 95 Overview of supplied attributes- XA image (Derived) from MR image* 123
*Table 96 Identifications of images* 124
*Table 97 Identifications of Store Monitor images* 124
*Table 98 Identifications of Reference images* 125
*Table 99 Identifications of Quant report images* 125
*Table 100 Identifications of Exam Protocol non-images* 125
*Table 101 Identifications of Exam Protocol as XA image* 125
*Table 102 Supported Matrix Sizes* 132
*Table 103 Printer Status Information* 136
*Table 104 Printer Status Information - Agfa* 137
*Table 105 Printer Status Information – Kodak (Imation)* 137
*Table 106 Printer Status Information – Kodak 190* 137
*Table 107 Printer Status Information – Kodak 2180/1120* 138
*Table 108 Printer Status Information – Codonics* 139
*Table 109 Additional DICOM Execution Status Infos* 139

# Table of Figures

*Figure 1* *Application Data Flow Diagram - Verification SCU/SCP* 13
*Figure 2* *Application Data Flow Diagram – Storage SCU/SCP* 16
*Figure 3* *Application Data Flow Diagram – Storage Commitment SCU* 27
*Figure 4* *Artis zee VC13 Application Data Flow Diagram – Query/Retrieve SCU* 31
*Figure 5* *Artis zee VC13 Application Data Flow Diagram – Query/Retrieve SCP* 31
*Figure 6* *DICOM Application Data Flow Diagram – Print SCU* 48
*Figure 7* *Artis zee VC13 Application Flow Diagram – Basic Worklist SCU* 56
*Figure 8* *Artis zee VC13 Application Flow Diagram – MPPS SCU* 65
*Figure 9* *Application Data Flow Diagram* 88
*Figure 10* *DICOM Information Model* 94
*Figure 11* *Image ordering – simple case* 127
*Figure 12* *Image ordering – with Reference images* 128
*Figure 13* *Image ordering – with Store Monitor images* 129
*Figure 14* *Image ordering – with Store Monitor and Quant images* 130

# 1 Introduction

## 1.1 Overview

The Conformance Statement describes the DICOM interface for the Siemens Artis zee VC13 in terms of part 2 of [DICOM].

This introduction describes the application's implemented DICOM functionality in general terms.

## 1.2 Scope and Field

The Artis zee VC13is a "*syngo*®-speaking[a]" Imaging Modality. The Artis zee VC13 is designed to be integrated into an environment of medical DICOM-based devices. The Artis zee VC13 DICOM network implementation acts as SCU and SCP for the DICOM Storage and Query/Retrieve services and as SCU for the DICOM Print, DICOM Basic Worklist, Storage Commitment and Modality Performed Procedure Step Services. Verification is supported in SCU (only via Service environment) and SCP role. Furthermore the handling of CD offline media is supported as a FSC, FSU and FSR.

| Software Name | SIEMENS Artis Product |
|---|---|
| Artis zee VC13 | *floor, ceiling, biplane, multi-purpose* |
| Artis zeego VC13 | *multi-axis* |

**Table 1 List of products applicable to this Conformance Statement**

## 1.3 Audience

This document is intended for hospital staff, health system integrators, software designers or implementers. It is assumed that the reader has a working understanding of DICOM.

## 1.4 Remarks

DICOM, by itself, does not guarantee interoperability. However, the Conformance Statement facilitates a first-level validation for interoperability between different applications supporting the same DICOM functionality as SCU and SCP, respectively.

This Conformance Statement is not intended to replace validation with other DICOM equipment to ensure proper exchange of information intended.

The scope of this Conformance Statement is to facilitate communication with Siemens and other vendors' Medical equipment. The Conformance Statement should be read and understood in conjunction with the DICOM 3.0 Standard [DICOM]. However, by itself it is not guaranteed to ensure the desired interoperability and a successful interconnectivity.

The user should be aware of the following important issues:

- The comparison of different conformance statements is the first step towards assessing interconnectivity between Siemens and non-Siemens equipment.
- Test procedures should be defined and tests should be performed by the user to validate the connectivity desired. DICOM itself and the conformance parts do not specify this.

[a] *syngo* is a registered trademark of Siemens AG

- The standard will evolve to meet the users' future requirements. Siemens is actively involved in developing the standard further and therefore reserves the right to make changes to its products or to discontinue its delivery.
- Siemens reserves the right to modify the design and specifications contained herein without prior notice. Please contact your local Siemens representative for the most recent product information.

## 1.5 Definitions, Terms and Abbreviations

Definitions, terms and abbreviations used in this document are defined within the different parts of the DICOM standard.

Additional Abbreviations and terms are as follows:

| | |
|---|---|
| AE | DICOM Application Entity |
| ASCII | American Standard Code for Information Interchange |
| DB | Database |
| DICOM | Digital Imaging and Communications in Medicine |
| DIMSE | DICOM Message Service Element |
| DIMSE-C | DICOM Message Service Element with Composite Information Objects |
| DSA | Digital Subtraction Angiography |
| IOD | DICOM Information Object Definition |
| ISO | International Standard Organization |
| NEMA | National Electrical Manufacturers Association |
| O | Optional Key Attribute |
| PDU | DICOM Protocol Data Unit |
| R | Required Key Attribute |
| RIS | Radiology Information System |
| RWA | Real-World Activity |
| SCP | DICOM Service Class Provider (DICOM server) |
| SCU | DICOM Service Class User (DICOM client) |
| SOP | DICOM Service-Object Pair |
| U | Unique Key Attribute |

## 1.6 References

[DICOM] Digital Imaging and Communications in Medicine (DICOM), NEMA PS 3.1-3.18, 2008

## 1.7 Structure

This Conformance Statement is subdivided into multiple Parts, which relate to individual documents needed to declare Conformance according to the requirements of "Part 2 - Conformance" of the DICOM Standard.

Those parts are:

- "Network Conformance Statement" for Network related Services
  - Storage - User/Provider (includes Verification - User/Provider)
  - Storage Commitment - User
  - Query/Retrieve - User/Provider
  - Basic Grayscale - User
  - Basic Worklist - User
  - Modality Performed Procedure Step - User

- "Media Conformance Statement"
- "Offline Media Conformance Statement" to support local archive media.
- A general Appendix.

# 2 Implementation Model Verification

The Artis zee VC13 DICOM Service Tool application requests Verification to verify the ability of a foreign DICOM application on a remote node to respond to DICOM messages.

Responding to Verification requests from remote nodes is handled by the Storage SCP application.

## 2.1 Application Data Flow Diagram

The Artis zee VC13 DICOM network implementation acts as SCU and via the Storage SCP application as SCP for the C-ECHO DICOM network service. The product target Operating System is Windows XP.

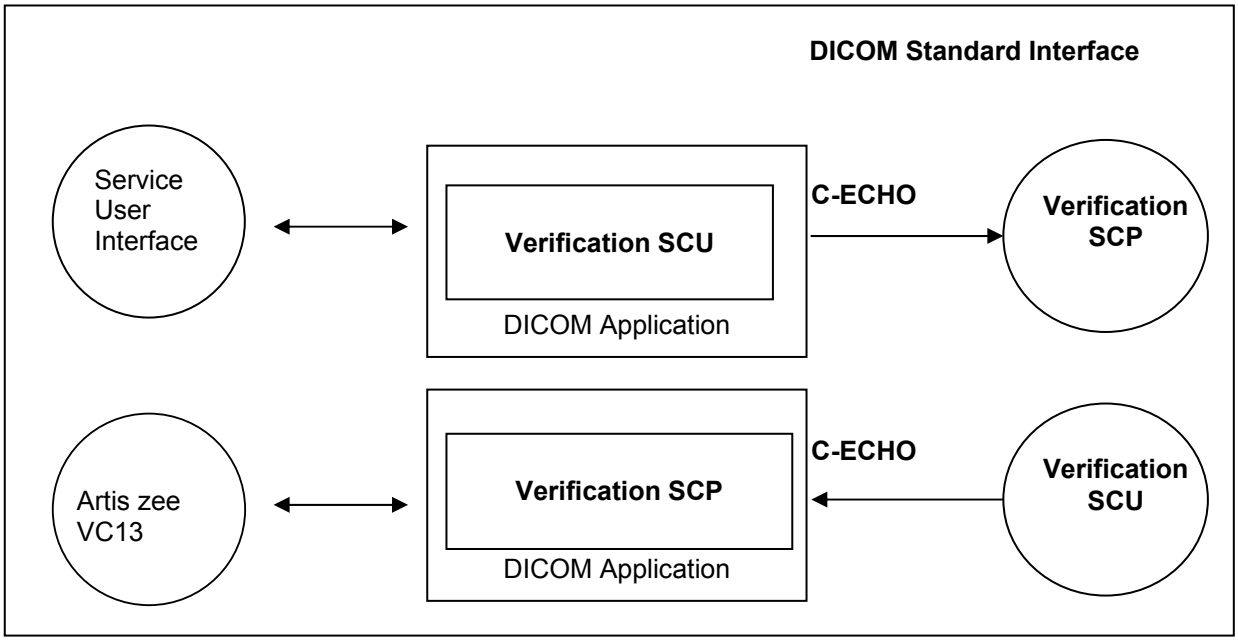


Figure 1 Application Data Flow Diagram - Verification SCU/SCP

## 2.2 Functional Definitions of Applications

The Artis zee VC13 DICOM Service Tool application opens an association when a “verification” of a remote application is requested during a configuration session. This can be done when entering new data for remote application configuration or to verify existing configuration data.

## 2.3 Sequencing of Real-World Activities

Newly entered data have to be saved first, before a “verification” of these data is possible.

# 3 Application Entity Specification Verification

## 3.1 Verification AE Specification

### 3.1.1 Association Establishment Policies

#### 3.1.1.1 General

The Artis zee VC13 DICOM Service Tool application attempts to open an association for verification request whenever the “verification” function is activated during network configuration of a remote DICOM application.

The Artis zee VC13DICOM application will accept association requests for verification.

#### 3.1.1.2 Number of Associations

The Artis zee VC13 DICOM Service Tool application initiates one association at a time to request verification.

The Artis zee VC13DICOM application is able to accept multiple associations at a time. It can handle up to 10 associations in parallel.

#### 3.1.1.3 Asynchronous Nature

The Artis zee VC13 DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

#### 3.1.1.4 Implementation Identifying Information

| | |
|---|---|
| Implementation Class UID | 1.3.12.2.1107.5.9.20000101 |
| Implementation Version Name | SIEMENS_SWFSYNGO |

Table 2 Implementation Identifying Information

### 3.1.2 Association Initiation Policy

The Artis zee VC13 DICOM Service Tool application attempts to initiate a new association for

- DIMSE C-ECHO

service operations.

#### 3.1.2.1 Associated Real-World Activity - Verification

#### 3.1.2.1.1 Associated Real-World Activity – Request Verification

The associated Real-World activity is a C-ECHO request initiated by Service and Configuration SW environment whenever a “verification” is requested. If an association to a remote Application Entity is successfully established, Verification with the configured AET is

requested via the open association. If the C-ECHO Response from the remote Application contains a status other than “Success” this will be indicated in the service environment and the association is closed.

#### 3.1.2.1.2 Proposed Presentation Contexts

The Artis zee VC13 DICOM application will propose Presentation Contexts as shown in the following table:

| Presentation Context Table – Verification SCU | | | | | |
|---|---|---|---|---|---|
| Abstract Syntax | | Transfer Syntax | | Role | Extended Negotiation |
| Name | UID | Name List | UID List | | |
| Verification | 1.2.840.10008.1.1 | Implicit VR Little Endian | 1.2.840.10008.1.2 | SCU | None |

Table 3 Proposed Presentation Contexts

#### 3.1.2.1.3 SOP Specific Conformance – Verification SCU

The Application conforms to the definitions of the Verification SCU in accordance to the DICOM Standard.

### 3.1.3 Association Acceptance Policy

As mentioned above, the Verification SCP is part of the Storage SCP – see section 5.1.3.

# 4 Implementation Model Storage

The Artis zee VC13 DICOM Application Entity both originates associations for Storage of DICOM Composite Information Objects in Remote Application Entities and accepts association requests for Storage from Remote Application Entities.

## 4.1 Application Data Flow Diagram

The Artis zee VC13 DICOM network implementation acts as SCU and SCP for the C-STORE DICOM network service and as SCP for the C-ECHO DICOM network service. The product target Operating System is Windows XP.

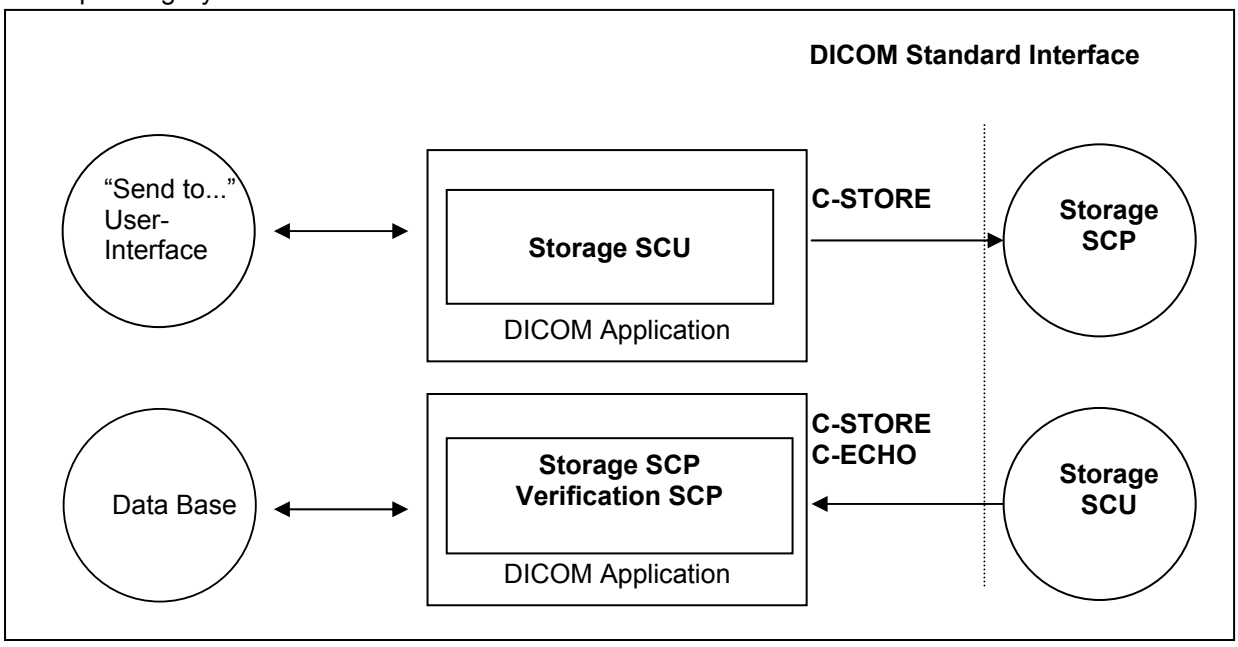


Figure 2 Application Data Flow Diagram – Storage SCU/SCP

## 4.2 Functional Definitions of Application Entities

The Storage SCU is invoked by the job control interface that is responsible for processing network archival tasks. The job consists of data describing the composite image objects selected for storage and the destination. An association is negotiated with the destination application entity and the image data is transferred using the C-STORE DIMSE-Service. Status of the transfer is reported to the job control interface.

The Storage SCP component of the Artis zee VC13 DICOM application is operating as background server process. It is running when the machine is powered on and waits for Storage association requests. Upon accepting an association with a negotiated Presentation Context it starts to receive the Composite Image Objects and imports them to local database. Verification requests will be processed and responded by Storage SCP component, too.

## 4.3 Sequencing of Real-World Activities

not applicable

# 5 Application Entity Specification Storage

## 5.1 Storage AEs Specification

The Artis zee VC13 Storage service class user/service class provider applications use one AE when initiating/receiving associations to/from remote DICOM nodes.

SIEMENS Artis zee VC13 DICOM products provide Standard Conformance to the following DICOM SOP Classes as an SCU:

| SOP Class Name | SOP Class UID |
|---|---|
| **X**-Ray **A**ngiographic Image Storage | 1.2.840.10008.5.1.4.1.1.12.1 |

Table 4 Supported SOP Classes as an SCU

SIEMENS Artis zee VC13 DICOM products provide Private Conformance to the following DICOM V3.0 conform private SOP Classes as an SCU:

| SOP Class Name | SOP Class UID |
|---|---|
| CSA Non-Image Storage | 1.3.12.2.1107.5.9.1 |

Table 5 Supported private SOP Classes as an SCU

SIEMENS Artis zee VC13 DICOM products provide Standard Conformance to the following DICOM V3.0 SOP Classes as an SCP:

| SOP Class Name | SOP Class UID |
|---|---|
| **C**omputed **T**omography Image Storage | 1.2.840.10008.5.1.4.1.1.2 |
| **M**agnetic **R**esonance Image Storage | 1.2.840.10008.5.1.4.1.1.4 |
| **X**-Ray **A**ngiographic Image Storage | 1.2.840.10008.5.1.4.1.1.12.1 |
| Verification | 1.2.840.10008.1.1 |

Table 6 Supported SOP Classes as an SCP

SIEMENS Artis zee VC13 DICOM products provide Private Conformance to the following DICOM-conform private SOP Classes as an SCP:

| SOP Class Name | SOP Class UID |
|---|---|
| CSA Non-Image Storage | 1.3.12.2.1107.5.9.1 |

**Table 7 Supported private SOP Classes as an SCP**

### 5.1.1 Association Establishment Policies

#### 5.1.1.1 General

The existence of a job queue entry with network destination or an internal trigger from processing a retrieve request will activate the DICOM Storage Application. An association request is sent to the destination AE and upon successful negotiation of a Presentation Context the transfer is started.

The default PDU size used will be 256 KB.

#### 5.1.1.2 Number of Associations

The Artis zee VC13 DICOM application initiates several associations at a time, one for each destination to which a transfer request is being processed in the active job queue list.

The Artis zee VC13 DICOM application is able to accept multiple associations at a time. It can handle up to 10 associations in parallel.

The number of Simultaneous DICOM associations can be configured via the Service-UI. The dialog can be found in Configuration / DICOM / General.

#### 5.1.1.3 Asynchronous Nature

The Artis zee VC13 DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

#### 5.1.1.4 Implementation Identifying Information

| | |
|---|---|
| Implementation Class UID | 1.3.12.2.1107.5.9.20000101 |
| Implementation Version Name | SIEMENS_SWFSYNGO |

Table 8 Implementation Identifying Information

### 5.1.2 Association Initiation Policy

If a job with network destination gets active in the job list or a retrieve sub-operation is processed the Artis zee VC13 DICOM application attempts to initiate a new association for

- DIMSE C-STORE

service operations.

#### 5.1.2.1 Associated Real-World Activity - Send

##### 5.1.2.1.1 Associated Real-World Activity – Send Image Objects to a Network Destination

The associated Real-World activity is a C-STORE request initiated by an internal daemon process triggered by a job with network destination or the processing of an external C-MOVE

retrieve request. If the process successfully establishes an association to a remote Application Entity, it will transfer each image one after another via the open association. If the C-STORE Response from the remote Application contains a status other than “Success” or “Warning”, the association is aborted.

#### 5.1.2.1.2 Proposed Presentation Context – Send Images

The Artis zee VC13 DICOM application will propose Presentation Contexts as shown in the following table:

| Presentation Context Table | | | | | |
|---|---|---|---|---|---|
| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg. |
| Name | UID | Name List | UID List | | |
| **X**-Ray **A**ngiographic Image | 1.2.840.10008.5.1.4.1.1.12.1 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>JPEG Lossless, Process 14 (selection value 1)<br>JPEG Lossy Baseline (Process 1)<br>JPEG Lossy Extended (Process 2 & 4)<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.4.70<br>1.2.840.10008.1.2.4.50<br>1.2.840.10008.1.2.4.51<br>1.2.840.10008.1.2.2 | SCU | None |
| CSA Non-Image | 1.3.12.2.1107.5.9.1 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCU | None |

Table 9 Proposed Presentation Context – Send Images

#### 5.1.2.1.3 SOP specific Conformance to Storage SOP classes

The Artis zee VC13 application will create XA IOD type images from image acquisition and post processing applications. Furthermore a private "Non-Image IOD" will be used to store numerical data and textual report results (e.g. Exam Protocol). It is possible to convert these reports to "XA Storage SOP Class" images during transfer.
The XA IOD will be a "Standard Extended XA Storage" SOP Class. For CT / MR imported/received images a conversion to a new XA image will be performed in order to enable viewing of those Instances on the Artis based System.

The Artis zee VC13 (DICOM) application will not change private attributes as long as no modification is done. During a “Store Monitor" or "Store Reference Image" operation all private attributes not defined within the Artis zee VC13 DICOM application will be removed when the new object instance is created.

For association and DIMSE level time-outs, please refer to Configuration section of this document.

##### 5.1.2.1.3.1 Optional Attributes

Data Dictionary of DICOM Type 2 and 3 IOD Attributes

Please see the related Image Object definition tables in the Annex A.4 for a list of all DICOM IOD attributes of type 2 and 3, which are encoded by the Artis zee VC13 applications.

##### 5.1.2.1.3.2 Specialized Information Object Definitions

The DICOM images created by Artis zee VC13 DICOM application conform to the DICOM IOD definitions (Standard extended IODs). But they will contain additional private elements, which have to be discarded by a DICOM system when modifying the image.

The DICOM nodes are responsible for data consistency when modifying images. All unknown private attributes have to be removed upon modification!

#### 5.1.2.1.3.3 Data Dictionary of applied private IOD Attributes

Please see “A.2” in the Annex for a list of possible private IOD attributes.

#### 5.1.2.1.3.4 Image Pixel Attribute Description for Grayscale Images

The Siemens Artis zee VC13 DICOM application supports the Monochrome2 Photometric Interpretation with the unsigned integer 16 bit grayscale pixel and graphic overlay format. The lower 12 bits are used for pixel and the higher 4 bits are used for the graphic overlay:

**Pixel plane**

- samples per pixel (attribute 0028, 0002) = 1
- photometric interpretation (attribute 0028,0004) = "MONOCHROME2"
- pixel representation (attribute 0028, 0103) = 0
- bits allocated (attribute 0028, 0100) = 8, 16
- bits stored (attribute 0028,0101) = 8, 10, 12
- high bit (attribute 0028,0102) = 7, 9, 11

**Overlay plane**

- overlay type (attribute 60xx, 0040) = "G"
- bits allocated (attribute 60xx, 0100) = 1
- bit position (attribute 60xx, 0102) = 0
- overlay data (attribute 60xx, 3000) = supported (always used with "bits allocated = 8")

#### 5.1.2.1.3.5 Private Information Object Definitions

To fulfill all application requirements the Artis zee VC13 DICOM implementation will use private IODs to store Data currently not defined in the DICOM Standard according to the DICOM information model. The privately defined IOD will contain all references to identify the Patient/ Study/Series/Images to which the related information is belonging to.

This private Information will include

- Complete Exam Protocol

All IOD used to store this private Information will be based on various Instances of the SIEMENS Non-Image IOD. Please see A.1 SIEMENS Private Non-Image IOD and A.5 Private Non-Image IOD in the Appendix for a detailed overview of the private IOD definition and the IOD tables for value encoding.

### 5.1.2.1.4 Associated Real-World Activity - Send Image Objects resized to a Network destination

In Local Service it is possible to configure each individual DICOM node (Store SCP) to receive Artis images resized to 512x512 or 1024x1024 matrix depending on image type, e.g. card images. The images in this case are "pre-processed" to be compliant to the Basic Cardiac Image definitions ($512^2$ Matrix with 8-Bits allocated).

#### 5.1.2.1.5 Proposed Presentation Contexts for resized images

The proposed Presentation Contexts for resized images are identical to those described in section 5.1.2.1.2 Proposed Presentation Context – Send Images.

#### 5.1.2.1.6 SOP Specific Conformance for resized images

The Artis zee VC13 System itself will create XA IOD type images from image acquisition and post processing applications. Furthermore a private "Non-Image IOD" will be used to store numerical data and textual report results (e.g. Exam Protocol). The XA IOD will be a “Standard Extended XA Storage” SOP Class. Please see the Appendix for detailed descriptions.

The Artis zee VC13 System supports a variety of matrix sizes (see Appendix). For better interoperability to different DICOM applications a conversion to 512x512 ("Resize 512") and 1024x1024 ("Resize 1024") matrix size is supported. Conversion is limited to reduction of Matrix Size and Pixel Depth and is restricted to be applied to “image-type” instances only.

"Resize 512" will allow conversion of any image that is displayed in the Artis zee VC13 viewing application to an image that conforms to the Basic Cardiac format.

Quant Report images are by nature 1024x1024 and will not be resized and are sent “as they are”.

The converted image is a temporary copy and therefore a new Instance UID is generated. The SOP Instance UID of the converted images will be created in a reproducible way by appending a "512" or "1024" to the original UID.

The conversion will generate a Pixel Matrix output that is described by the following Attribute values:

| Tag | DICOM Attribute | Attribute value (Resize 512) | Attribute value (Resize 1024) |
|---|---|---|---|
| [0028,0010] | Rows | **512** | **1024** |
| [0028,0011] | Columns | **512** | **1024** |
| [0028,0100] | Bits allocated | **8** | **16** |
| [0028,0101] | Bits Stored | **8** | **12** |
| [0028,0102] | High Bit | **7** | **11** |

Table 10 Resized images attributes

In order to preserve integrity of the data with respect to the original Matrix Size and Pixel Depth, the following attributes will be adapted accordingly for the resulting image:

- [0018,1602] Shutter Left Vertical Edge
- [0018,1604] Shutter Right Vertical Edge
- [0018,1606] Shutter Upper Horizontal Edge
- [0018,1608] Shutter Lower Horizontal Edge

- [0018,1702] Collimator Left Vertical Edge
- [0018,1704] Collimator Right Vertical Edge
- [0018,1706] Collimator Upper Horizontal Edge
- [0018,1708] Collimator Lower Horizontal Edge
- [0018,1720] Vertices of the Polygonal Collimator
- [0018,1164] Imager Pixel Spacing
- [0028,1050] Window Center
- [0028,1051] Window Width
- [0028,3002] MOD LUT Descriptor
- [0028,3006] MOD LUT Data
- [6000,0010] Overlay Rows
- [6000,0011] Overlay Columns
- [6000,3000] Overlay Data
- private data attributes

### 5.1.3 Association Acceptance Policy

The Artis zee VC13 DICOM application attempts to accept a new association for

- DIMSE C-ECHO
- DIMSE C-STORE

service operations. Any Information Objects transmitted on that association will be checked on conformance and stored in the database if check was successful.

#### 5.1.3.1 Associated Real-World Activity - Receive

##### 5.1.3.1.1 Associated Real-World Activity – Receiving Images from a Remote Node

The daemon receiving process will accept an association and will receive any images transmitted on that association and will store the images on disk in the own database if the conformance check is performed successfully.

##### 5.1.3.1.2 Accepted Presentation Context – Receiving Images

The Artis zee VC13 DICOM storage provider will only accept MONOCHROMEx encoded images.

Color encoded images (RGB or Palette Color) are not supported.

The Artis zee VC13 DICOM application will accept Presentation Contexts as shown in the following table:

| Presentation Context Table | | | | | |
|---|---|---|---|---|---|
| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg. |
| Name | UID | Name List | UID List | | |
| **C**omputed **T**omography Image | 1.2.840.10008.5.1.4.1.1.2 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>JPEG Lossless, Process 14 (selection value 1)<br>JPEG Lossy Baseline (Process 1) ***1**<br>JPEG Lossy Extended ***1** (Process 2 & 4)<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.4.70<br>1.2.840.10008.1.2.4.50<br>1.2.840.10008.1.2.4.51<br>1.2.840.10008.1.2.2 | SCP | None |
| **M**agnetic **R**esonance Image | 1.2.840.10008.5.1.4.1.1.4 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>JPEG Lossless, Process 14 (selection value 1)<br>JPEG Lossy Baseline (Process 1) ***1**<br>JPEG Lossy Extended ***1** (Process 2 & 4)<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.4.70<br>1.2.840.10008.1.2.4.50<br>1.2.840.10008.1.2.4.51<br>1.2.840.10008.1.2.2 | SCP | None |
| **X**-Ray **A**ngiographic Image | 1.2.840.10008.5.1.4.1.1.12.1 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>JPEG Lossless, Process 14 (selection value 1)<br>JPEG Lossy Baseline (Process 1) ***1**<br>JPEG Lossy Extended ***1** (Process 2 & 4)<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.4.70<br>1.2.840.10008.1.2.4.50<br>1.2.840.10008.1.2.4.51<br>1.2.840.10008.1.2.2 | SCP | None |
| CSA Non-Image Storage | 1.3.12.2.1107.5.9.1 | Implicit VR Little Endian<br>Explicit VR Big Endian<br>Explicit VR Little Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCP | None |
| Verification | 1.2.840.10008.1.1 | Implicit VR Little Endian<br>Explicit VR Big Endian<br>Explicit VR Little Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCP | None |

**Table 11 Proposed Presentation Context – Receiving Images**

### 5.1.3.1.3 SOP-specific Conformance Statement – Receiving Images

The Artis zee VC13 DICOM application conforms to the Full Storage Class at Level **2**.

Upon successfully receiving a C-STORE-RQ, the Siemens Artis zee VC13 DICOM receiver performs a plausibility test on the received image and checks the availability of system resources. In the event of a successful C-STORE operation, the image has successful been written on disk in the Siemens Artis zee VC13 image format. For Private Attributes of VR=SQ only a nesting level of one is supported. This means that Private Sequences containing another Sequence will be removed from the image header during Storage.

The Artis zee VC13 DICOM application returns the status SUCCESS upon successful operation, otherwise one of the following status codes is returned and the association is aborted:

- Refused (A700):
  This error status indicates a lack of Resources (e.g. not enough disk space) on the Artis zee VC13 modality.
- Invalid Dataset (0xA900 or 0xC000):
  An error occurred while processing the image which makes it impossible to proceed. The image will not be stored and the association is aborted. The dataset may not contain one of

the Attributes “Study Instance UID”, “Series Instance UID” or “SOP Instance UID”, or one of them might have an invalid value.

- Processing Error (0110):
  An error occurred while processing the image, which makes it impossible to proceed.

**Attention!** Only after sending the response, the image will be saved into the database. If during this operation an error occurs, the association will be aborted. This implies that a C-STORE-RSP with status SUCCESS does not mean that the image was successfully stored into the database.

If an image instance is received that is identified by a SOP Instance UID which is already used by an Instance stored in database then the actual received image will be discarded. The existing Instance is not superseded.

#### 5.1.3.1.3.1 Optional Attributes acceptance criterion - applied defaults

Upon receiving IOD other than created by the Artis zee VC13 DICOM application a check for conformity is done and with successful completion the IOD is accepted for storage. Hereby defaults will be set when optional attributes are encountered with "no value" coding. Please see the following tables for details.

| Attribute Name | Tag | Default Value |
|---|---|---|
| Window Center | [0028,1050] | Open window, e.g. bits stored=12 -> window center=2048 |
| Window Width | [0028,1051] | Open window, e.g. bits stored=12 -> window width=4095 |

Table 12 Attributes with applied defaults

The following sections will differentiate the attribute contents required for Image Viewing. The Artis zee VC13 DICOM application supports more formats for Storage of Images than Viewing.

#### 5.1.3.1.3.2 Image Pixel Attribute Acceptance Criterion for Grayscale Images - Viewing

The Artis zee VC13 Viewing application accepts the MONOCHROME2 photometric interpretation pixel format and graphic overlay with unsigned integer and 8 or 16 bits allocated. Accepted values:

- Pixel plane
  - samples per pixel (attribute 0028, 0002) = 1
  - photometric interpretation (attribute 0028,0004) = “MONOCHROME2”
  - pixel representation (attribute 0028, 0103) = 0
  - bits allocated (attribute 0028, 0100) = 8, 16
  - bits stored (attribute 0028,0101) = 8, 10, 12
  - high bit (attribute 0028,0102) = 7, 9, 11
  - only aspect ratio 1:1 is supported
  - number of rows (0028,0010) and columns (0028,0011) = 512 or 1024
- Overlay plane
  - overlay type (attribute 60xx, 0040) = “G”
  - bits allocated (attribute 60xx, 0100) = 16

- bit position (attribute 60xx, 0102) = 12, 13, 14, 15 (only bits above high bit permitted)
- Graphic Overlay will be shifted to fill Overlay Planes from Bit 12 and consecutive.

- Overlay plane
  - overlay type (attribute 60xx, 0040) = “G”
  - bits allocated (attribute 60xx, 0100) = 1
  - bit position (attribute 60xx, 0102) = 0
  - overlay data (attribute 60xx, 3000) = supported

Additionally all matrix sizes (rows and columns) generated by the Artis zee VC13 are supported. For a complete list, please refer to Annex A.9.

Only Rectangular and Circular Shutter Shape is supported in this version. Images containing other Shutter Shapes will be displayed w/o shutter.

With multi-frame images the Overlay Graphic is only supported as replication of the 1st frame's overlay data.

#### 5.1.3.1.4 Presentation Context Acceptance Criterion

The Artis zee VC13 DICOM application will accept any number of verification or storage SOP classes that are listed above. The number of presentation contexts accepted is limited to the maximum of 127 (DICOM limit). In the event that the Artis zee VC13DICOM application runs out of resources, it will reject the association request.

#### 5.1.3.1.5 Transfer Syntax Selection Policies

The Artis zee VC13 DICOM application currently supports

- the Implicit VR Little Endian, the Explicit VR Little Endian and Explicit VR Big Endian Transfer Syntaxes
- the JPEG Lossless Non-hierarchical Transfer Syntax
- the JPEG Baseline and JPEG Extended Transfer Syntaxes (JPEG Lossy).

Any proposed presentation context including one of these Transfer Syntaxes will be accepted. Any proposed presentation context that does not include one of these Transfer Syntaxes will be rejected.

The order of preference in accepting Transfer Syntaxes within Presentation Contexts or Presentation Contexts with single Transfer Syntaxes is:

1. JPEG Lossy Extended
2. JPEG Lossless non-hierarchical
3. JPEG Lossy Baseline
4. Explicit VR Little Endian
5. Explicit VR Big Endian
6. Implicit VR Little Endian

With Implicit VR Little Endian Transfer Syntax the Artis zee VC13 DICOM application will remove any Private Attributes not known to the application. Decision on removal of a Private Element is done if there is NO entry in the attribute-dictionary of the Artis zee VC13 DICOM application.

Therefore any Explicit VR Transfer Syntax shall preferably be used by the Storage SCUs when sending Composite Image Instances to the Artis zee VC13 DICOM application.

# 6 Implementation Model Storage Commitment

The Storage Commitment service class defines an application-level class of service which facilitates the commitment to storage. It performs an additional task of commitment of composite objects apart from the network based storage of images as defined by the Storage Service class. The Artis zee VC13 DICOM implementation supports the Storage Commitment Push Model as SCU.

## 6.1 Application Data Flow Diagram

The Artis zee VC13 DICOM network implementation acts as SCU for the Storage Commitment Push Model Service using the Storage Commitment Service Class. The product target Operating System is Windows XP.

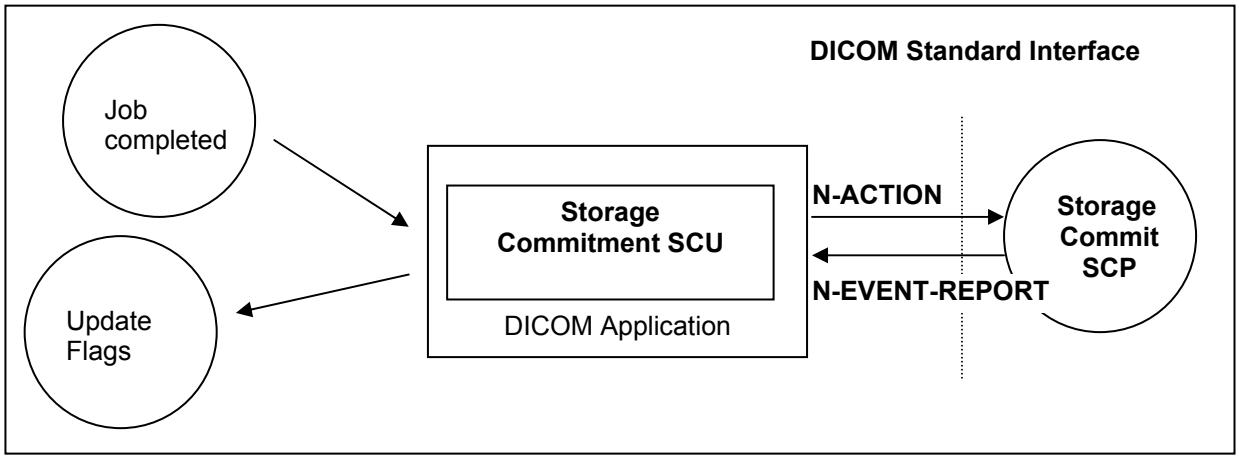


Figure 3 Application Data Flow Diagram – Storage Commitment SCU

## 6.2 Functional Definitions of Application Entities

If configured, the Artis zee VC13 DICOM Application will create a Storage Commitment Push Model Identifier for each successfully completed send job. Then a Storage Commit Request is triggered. Depending on configuration, the Artis zee VC13 DICOM application will keep the association open for responses with a configurable time-out, or closes the association and expects responses on a different association that has to be established by the remote Storage Commitment SCP.

The commitment status derived from the related trigger response will be indicated in the related Status Flags of the related entity. It is possible to create triggers (“auto rules”) from this event.

The Transaction UIDs of the pending commitment request are kept “open” for a configurable amount in time (default: 1h). If the “open time” for a pending commitment request has elapsed w/o a related response from the provider, the Transaction UID is removed and the related entities are indicated as “commit failed”.

In any case, commitment will only be requested for previously and successfully sent images.

## 6.3 Sequencing of real World Activities

The Storage Commitment trigger is automatically derived from the successful completion of a Send Job.

# 7 AE Specification Storage Commitment

## 7.1 Storage Commitment AE Specification

SIEMENS Artis zee VC13 DICOM application provides Standard Conformance to the following DICOMV3.0 SOP Class as an SCU:

| SOP Class Name | SOP Class UID |
|---|---|
| Storage Commitment Push Model | 1.2.840.10008.1.20.1 |

Table 13 Storage Commitment SOP Class supported

### 7.1.1 Association Establishment Policies

#### 7.1.1.1 General

With a Send Job successfully completed, the DICOM application will generate an Storage Commitment Identifier which references to all Instances of the processed job. The Commit Request is then sent over a single opened association. The Artis zee VC13 will wait for Status responses of the Storage Commitment Request. If the Provider accepts the Storage Commitment with Success Status, the generated Transaction UID, together with study identification data and a time-stamp, is kept. Depending on configuration, the association is closed when the configured time-out has elapsed or a response was received before. If the association is closed before a response was received, the response is then expected on a different association. Multiple Storage Commitment Requests can be pending.

The default PDU size used will be 256 KB.

#### 7.1.1.2 Number of Associations

The Artis zee VC13 DICOM application initiates several associations at a time, one for each storage commitment request being processed.

#### 7.1.1.3 Asynchronous Nature

The Artis zee VC13 DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

#### 7.1.1.4 Implementation Identifying Information

| | |
|---|---|
| Implementation Class UID | 1.3.12.2.1107.5.9.20000101 |
| Implementation Version Name | SIEMENS_SWFSYNGO |

Table 14 Implementation Identifying Information

### 7.1.2 Association Initiation Policy

The Artis zee VC13 DICOM Application Entity acts as a Service Class User (SCU) for the

- Storage Commitment Push Model Service Class (to request commitment for storage of instances previously sent).

  To do so, the Artis zee VC13 will issue a

- N-ACTION DIMSE to request commitment

### 7.1.2.1 Real World Activity – Storage Commitment

#### 7.1.2.1.1 Associated Real-World Activity - Job Completed

The Artis zee VC13 Storage Commitment application sends the commit request (N-ACTION-RQ) message and waits for acceptance of this request (N-ACTION-RSP). After receiving this, the transaction is marked as “waiting”.

Depending on a configuration value, the association will then be closed or kept open. In the first case, there is another configurable timeout giving the number of hours (h) and minutes (m) (by default 1h:0m) to wait for the corresponding commit response (N-EVENT-REPORT). In the second case, this time is the (also configurable) time-out for the association. For both cases, if the commit response (N-EVENT-REPORT) does not arrive during the configured time, the transaction will be marked as failed. The Artis zee VC13 does not resend objects from a failed Storage Commitment result in any case.

If the commit response (N-EVENT-REPORT) received has the status of “complete - failure exists”, the transaction is marked as failed, else the transaction is marked as “completed”; In both cases, a message is shown to the user.

#### 7.1.2.1.2 Proposed Presentation Contexts - Job Completed

The Artis zee VC13 DICOM application will propose Presentation Contexts as shown in the following table:

| Presentation Context Table | | | | | |
|---|---|---|---|---|---|
| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg. |
| Name | UID | Name List | UID List | | |
| Storage Commitment Push Model | 1.2.840.10008.1.20.1 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCU | None |

Table 15 Proposed Presentation contents – request Storage Commitment

#### 7.1.2.1.3 SOP Specific Conformance Statement- Job Completed

Storage Commitment is supported for all the SOP class UIDs mentioned in Chapter 5.1.3.1.2.

The Referenced Study Component Sequence is not supported.

Storage Media File-Set ID and UID Attributes is not supported in the commitment request (N-ACTION primitive) invoked by the Storage Commitment SCU.

#### 7.1.2.1.4 Associated Real-World Activity - Update Flags

The Artis zee VC13 Storage Commitment DICOM Application has sent a Storage Commitment Request and, being configured to receive response on a separate association, has closed the association, and now it gets an association request from the Storage Commitment SCP that want to send the results. The Artis zee VC13 DICOM application will await Storage commitment

Notification triggers. Any incoming Notification will be checked for validity, that is, if the related Transaction UID is still part of the Pending Request Queue.

If the Notification is valid, the Notification Event Information is evaluated and the related Instances marked with the related status. The over-all Commit Status of the higher Information Entities is derived from propagation of the States of all Image entities included in a study.

The Status Flags directly affected by Storage Commitment results and indicated in the different entities of the Patient Browser list can be one of

- "AC" or "SC" - Successful Commitment, A means archived to configured Archive destination, whereas S means sent to any other destination
- "Af" of "Sf" - Commitment failed.
- "A?" or "S?" - Commitment request is sent, response is pending.

In case of failure the user has to repeat the transfer of images to the Archive destination. Another Storage Commitment will be performed after sending is completed successfully.

#### 7.1.2.1.5 Accepted Presentation Contexts - Update Flags

The Siemens Artis zee VC13 DICOM application will accept Presentation Contexts as shown in the following table:

| Presentation Context Table | | | | | |
|---|---|---|---|---|---|
| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg. |
| Name | UID | Name List | UID List | | |
| Storage Commitment Push Model | 1.2.840.10008.1.20.1 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCU | None |

Table 16 Accepted Presentation contents – request Storage Commitment

#### 7.1.2.1.6 SOP-specific Conformance Statement - Update Flags

If the Commitment response (N-EVENT-REPORT) received has the status of "complete - failure exists", the transaction is marked as failed, else the transaction is marked as "completed"; In both cases, a message is shown to the user.

The related status flags are set for the committed images in the local database.

For images sent in resized format, the flag will be set for the original images still available on the system.

The Artis zee VC13 DICOM application will not support the Storage Media File Set ID attributes.

# 8 Implementation Model Query / Retrieve

The query/retrieve service class defines an application-level class of services which facilitates the management of images and patient data against the well-defined information model of DICOM and allows a DICOM AE to retrieve images from a remote DICOM node or to request a remote DICOM AE to initiate a transfer of images to another DICOM AE. The Artis zee VC13 DICOM query/retrieve application supports the query/retrieve services to act as SCU and SCP.

## 8.1 Application Data Flow Diagram

The Artis zee VC13 DICOM network implementation acts as SCU and SCP for the query/retrieve network service. The product target Operating System is Windows XP.

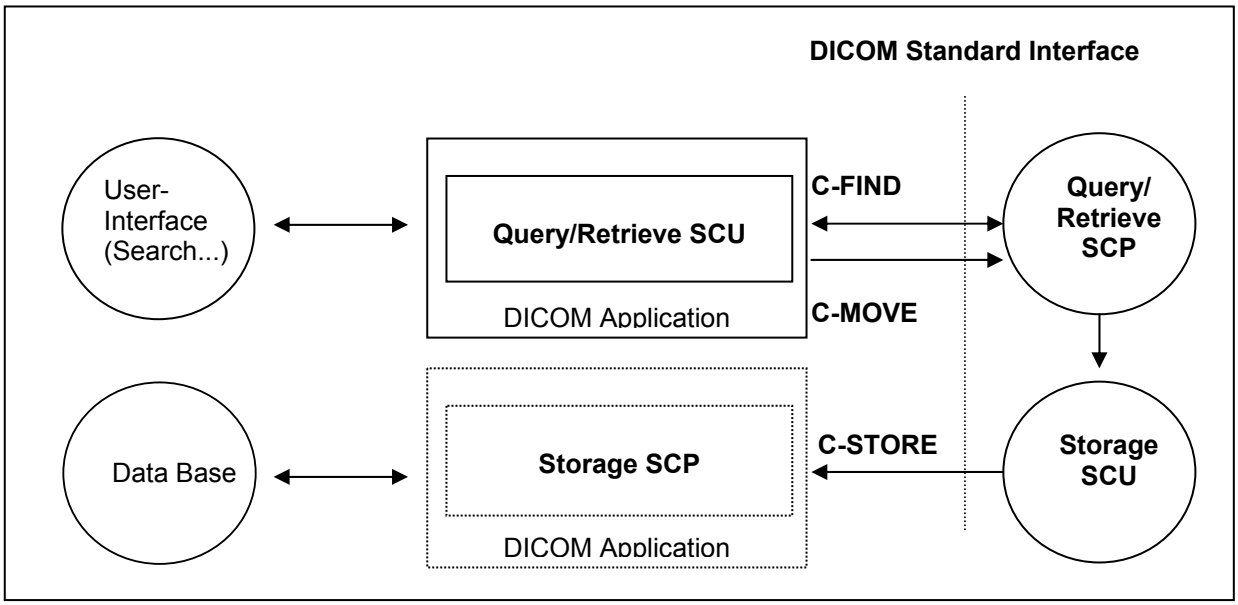


**Figure 4 Artis zee VC13 Application Data Flow Diagram – Query/Retrieve SCU**

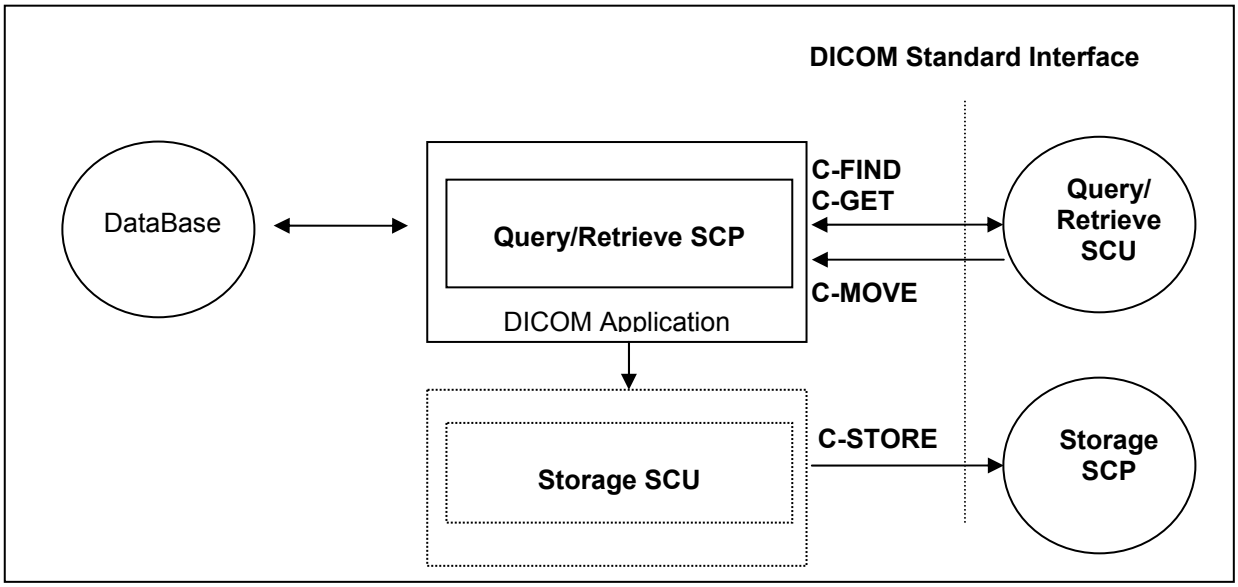


**Figure 5 Artis zee VC13 Application Data Flow Diagram – Query/Retrieve SCP**

## 8.2 Functional Definitions of Application Entities

The Artis zee VC13 DICOM Query/Retrieve SCU requests the remote query/retrieve SCP to perform a search and match to the keys specified in the request in order to display the results in the Artis zee VC13 user interface. Depending on user action (Import) the Artis zee VC13 DICOM SCU sends a C-MOVE DIMSE service to initiate a C-STORE sub-operation on the SCP to start an image transfer from remote Storage SCU (running on Query/Retrieve SCP) to the Artis zee VC13 Storage SCP.

The Artis zee VC13 DICOM query/retrieve SCP responds to C-FIND DIMSE services from remote SCU applications. Depending on further remote request, a C-GET or a C-MOVE involves the Artis zee VC13 DICOM query/retrieve SCP application to initiate a C-STORE association (by triggering the own Storage SCU) to send image objects to a remote Storage SCP.

All components of the DICOM query/retrieve SCP application are operating as background server processes. They are running when the machine is powered on and respond to queries based on the records stored in the database.

## 8.3 Sequencing of Real-World Activities

Retrieve of images is only possible if results from a previous “Search...” operation are available and those entities can be selected for “Import”.

# 9 Application Entity Specification Query/Retrieve

## 9.1 Query/Retrieve Service AEs Specification

The Query/Retrieve SCU requests that the remote SCP performs a match of all keys specified in the request, against the information in its database and the identified images will be moved over a different (C-MOVE) storage association.

The Query/Retrieve SCP responds to queries based on the records based on its database and images will be sent to the requesting SCU or to a different storage destination.

SIEMENS Artis zee VC13 DICOM products provide Standard Conformance to the following DICOM V3.0 SOP Classes as SCU:

| SOP Class Name | SOP Class UID |
|---|---|
| Patient Root Query/Retrieve Information Model - FIND | 1.2.840.10008.5.1.4.1.2.1.1 |
| Patient Root Query/Retrieve Information Model - MOVE | 1.2.840.10008.5.1.4.1.2.1.2 |
| Study Root Query/Retrieve Information Model - FIND | 1.2.840.10008.5.1.4.1.2.2.1 |
| Study Root Query/Retrieve Information Model - MOVE | 1.2.840.10008.5.1.4.1.2.2.2 |
| Patient/Study Only Query/Retrieve Information Model - FIND | 1.2.840.10008.5.1.4.1.2.3.1 |
| Patient/Study Only Query/Retrieve Information Model - MOVE | 1.2.840.10008.5.1.4.1.2.3.2 |

Table 17 Supported SOP Classes as SCU

SIEMENS Artis zee VC13 DICOM products provide Standard Conformance to the following DICOM V3.0 SOP Classes as an SCP:

| SOP Class Name | SOP Class UID |
|---|---|
| Patient Root Query/Retrieve Information Model - FIND | 1.2.840.10008.5.1.4.1.2.1.1 |
| Patient Root Query/Retrieve Information Model - MOVE | 1.2.840.10008.5.1.4.1.2.1.2 |
| Patient Root Query/Retrieve Information Model - GET | 1.2.840.10008.5.1.4.1.2.1.3 |
| Study Root Query/Retrieve Information Model - FIND | 1.2.840.10008.5.1.4.1.2.2.1 |
| Study Root Query/Retrieve Information Model - MOVE | 1.2.840.10008.5.1.4.1.2.2.2 |
| Study Root Query/Retrieve Information Model - GET | 1.2.840.10008.5.1.4.1.2.2.3 |
| Patient/Study Only Query/Retrieve Information Model - FIND | 1.2.840.10008.5.1.4.1.2.3.1 |
| Patient/Study Only Query/Retrieve Information Model – MOVE | 1.2.840.10008.5.1.4.1.2.3.2 |
| Patient/Study Only Query/Retrieve Information Model - GET | 1.2.840.10008.5.1.4.1.2.3.3 |

Table 18 Supported SOP Classes as SCP

**Note:** See also the Storage DICOM Conformance Statement of the Artis zee VC13 DICOM application to compare for conformance of the C-STORE sub-operation generated by the C-GET or C-MOVE DIMSE services. Furthermore compare the supported Storage Service SOP classes

described in the Storage DICOM Conformance Statement of the Modality to which the images shall be transferred to.

### 9.1.1 Association Establishment Policies

#### 9.1.1.1 General

With the “Search...” function the query data are input and the DICOM query/retrieve application is started. A query request will be sent out to one remote node that can be selected from a list of configured Query Providers and the response data will be displayed for the user. Upon request (Import), the retrieval of selected items is initiated.

The default PDU size used will be 256 KB.

#### 9.1.1.2 Number of Associations

The Artis zee VC13 DICOM application initiates one association for each query request being processed to a remote node. The maximum number of active associations is configurable.

The Artis zee VC13 DICOM application is able to accept multiple associations at a time. It can handle up to 10 associations in parallel.

#### 9.1.1.3 Asynchronous Nature

The Artis zee VC13 DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

#### 9.1.1.4 Implementation Identifying Information

| | |
|---|---|
| Implementation Class UID | 1.3.12.2.1107.5.9.20000101 |
| Implementation Version Name | SIEMENS_SWFSYNGO |

Table 19 Implementation Identifying Information

### 9.1.2 Association Initiation Policy

The query user interface will request the query-data from the user and triggers one C-FIND request to the selected remote node. The response data will be displayed in the query UI for further data navigation.

When requesting Import of related items the browser requests the retrieve application to send a C-MOVE request to the related remote node. Images will then be received by the Storage SCP as described in the related section.

The query/retrieve operation can be canceled at any time by a respective C-FIND-CANCEL or C-MOVE-CANCEL.

#### 9.1.2.1 Real World Activity - Find SCU

##### 9.1.2.1.1 Associated Real-World Activity - Find SCU “Search”

The associated Real-World activity is to fill out a query form with search data and pass it as query to the network application which issues a C-FIND over a previously built association. The remote SCP will respond with related data-entries that will be passed to a browser application. When data transfer is finished the association is closed.

#### 9.1.2.1.2 Proposed Presentation Contexts - Find SCU

The Artis zee VC13 DICOM application will propose Presentation Contexts as shown in the following table:

| Presentation Context Table | | | | | |
|---|---|---|---|---|---|
| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg. |
| Name | UID | Name List | UID List | | |
| Patient Root Query/Retrieve Model - FIND | 1.2.840.10008.5.1.4.1.2.1.1 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCU | None |
| Study Root Query/Retrieve Model – FIND | 1.2.840.10008.5.1.4.1.2.2.1 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCU | None |
| Patient/Study Only Query/Retrieve Model – FIND | 1.2.840.10008.5.1.4.1.2.3.1 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCU | None |

Table 20 Proposed Presentation Contexts - Find SCU

It is configurable which of the two query models (or both) are to be used by the Artis zee VC13 DICOM Query SCU application. If both Abstract Syntaxes are configured, The C-FIND SCU will use the Patient Root Model only for C-FIND requests on PATIENT level. For all other levels it will use the STUDY root model.

#### 9.1.2.1.3 Conformance Statement - Find SCU

The Artis zee VC13 DICOM Query/Retrieve SCU supports hierarchical queries with all mandatory search keys. The interactive querying of attributes on IMAGE level is supported by the Query SCU, hence but no search criteria can be entered. So image level is always queried with a fixed list of "universal(Null)" values.

The following table describes the search keys for the different query models that the SCU supports. Matching is either wildcard, which means that the user can supply a string containing wildcards, or universal, which means that the attribute is requested as return value.

| Attribute name | Tag | Type | Matching | User input | return value display |
|---|---|---|---|---|---|
| **Patient Level** [a] | | | | | |
| Patient Name | (0010,0010) | R | Wildcard[b] | enter value | yes |
| Patient ID | (0010,0020) | U | Wildcard | enter value | yes |
| Patient's Birth date | (0010,0030) | O | universal (Null) | enter value | yes |
| Patient's Sex | (0010,0040) | O | universal (Null) | enter value | yes |
| Number of Patient related Studies | (0020,1200) | O | universal (Null) | - | yes[a] |

a Patient Root Information Model only
b Always a "*" is appended to the user-supplied string

| Attribute name | Tag | Type | Matching | User input | return value display |
|---|---|---|---|---|---|
| Number of Patient related Series | (0020,1202) | O | universal (Null) | - | no |
| Number of Patient related Instances | (0020,1204) | O | universal (Null) | - | no |
| **Study Level** | | | | | |
| Patient Name [d] | (0010,0010) | R | Wildcard[b] | enter value | yes |
| Patient ID | (0010,0020) | R | Wildcard[b] | enter value | yes |
| Patient's Birth date [d] | (0010,0030) | O | universal (Null) | enter value | yes |
| Patient's Sex [d] | (0010,0040) | O | universal (Null) | enter value | yes |
| Study Instance UID | (0020,000D) | U | single value | - | yes |
| Study ID | (0020,0010) | R | universal (Null) | enter value | yes |
| Study Date | (0008,0020) | R | universal (Null) | enter value | yes |
| Study Time | (0008,0030) | R | universal (Null) | - | yes |
| Accession Number | (0008,0050) | R | universal (Null) | - | yes |
| Study Description | (0008,1030) | O | universal (Null) | - | yes |
| Referring Physician's Name | (0008,0090) | O | universal (Null) | - | yes |
| Name of Physician Reading Study | (0008,1060) | O | universal (Null) | - | yes |
| Modalities in Study | (0008,0061) | O | universal (Null) | - | yes |
| Storage Media File-Set ID | (0008,0130) | O | universal (Null) | - | no |
| Retrieve AE Title | (0008,0054) | O | universal (Null) | - | no |
| Number of Study related Series | (0020,1206) | O | universal (Null) | - | yes |
| Number of Study related Instances | (0020,1208) | O | universal (Null) | - | no |
| **Series Level** | | | | | |
| Series Instance UID | (0020,000E) | U | single value | - | yes |
| Series Number | (0020,0011) | R | universal (Null) | - | yes |
| Modality | (0008,0060) | R | universal (Null) | enter value | yes |
| Series Date | (0008,0021) | O | universal (Null) | - | yes |
| Series Time | (0008,0031) | O | universal (Null) | - | yes |
| Series Description | (0008,103E) | O | universal (Null) | enter value | yes |
| Body Part Examined | (0018,0015) | O | universal (Null) | enter value | yes |
| Performing Physician | (0008,1050) | O | universal (Null) | enter value | yes |
| Storage Media File-Set ID | (0008,0130) | O | universal (Null) | - | yes |
| Retrieve AE Title | (0008,0054) | O | universal (Null) | - | yes |
| Protocol Name | (0018,1030) | O | universal (Null) | - | no |

c Implicitly visualized in the UI if no study and series search attributes have been entered
d Study Root model only

| Attribute name | Tag | Type | Matching | User input | return value display |
|---|---|---|---|---|---|
| Perf. Procedure Step Start Date | (0040,0244) | O | universal (Null) | - | yes |
| Perf. Procedure Step Start Time | (0040,0245) | O | universal (Null) | - | yes |
| Request Attribute Sequence | (0040,0275) | O | universal (Null) | - | yes |
| > Requested Procedure ID | (0040,1001) | O | universal (Null) | - | yes |
| > Scheduled Procedure ID | (0040,0009) | O | universal (Null) | - | yes |
| Number of Series related Instances | (0020,1209) | O | universal (Null) | - | yes |
| **Image Level** | | | | | |
| SOP Instance UID | (0008,0018) | U | single value | - | no |
| Image Number | (0020,0013) | R | universal (Null) | - | yes |
| Storage Media File-Set ID | (0008,0130) | O | universal (Null) | - | no |
| Retrieve AE Title | (0008,0054) | O | universal (Null) | - | no |
| Instance Date | (0008,0023) | O | universal (Null) | - | no |
| Instance Time | (0008,0033) | O | universal (Null) | - | no |
| Number of Frames | (0028,0008) | O | universal (Null) | - | yes |
| Image Comments | (0020,4000) | O | universal (Null) | - | no |

Table 21 Search keys for Query models - Find SCU

The Find SCU interprets following status codes:

| Service Status | Meaning | Protocol Codes | Related Fields |
|---|---|---|---|
| Refused | Out of Resources | A700 | (0000,0902) |
| Failed | Identifier does not match SOP Class | A900 | (0000,0901) (0000,0902) |
| | Unable to process | Cxxx | (0000,0901) (0000,0902) |
| Cancel | Matching terminated due to Cancel request | FE00 | None |
| Success | Matching is complete - No final Identifier is supplied | 0000 | None |
| Pending | Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys | FF00 | Identifier |
| | Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this identifier | FF01 | Identifier |

Table 22 C-FIND response status

### 9.1.2.2 Real-World Activity – Move SCU

#### 9.1.2.2.1 Associated Real-World Activity – Move SCU "Import"

When selecting a data entry in the Query UI and activate the "Import" function, a retrieval request is passed to the archival application which issues a C-MOVE service according to the Patient Root or Study Root query model. (The Storage Service Class Conformance Statement describes the C-STORE service, which is generated by processing the C-MOVE service.)

The transferred image data are processed as described in the storage class SCP descriptions.

The possibility to request the remote C-MOVE provider (remote application that responded to the C-FIND) to move data to an application entity other than the C-MOVE SCU (the Artis zee VC13 DICOM application) is not used.

C-MOVE operation on Patient Level is not supported by the Query UI.

#### 9.1.2.2.2 Proposed Presentation Contexts - Move SCU "Import"

The Artis zee VC13 DICOM application will propose Presentation Contexts as shown in the following table:

| Presentation Context Table | | | | | |
|---|---|---|---|---|---|
| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg. |
| Name | UID | Name List | UID List | | |
| Patient Root Query/Retrieve Model – MOVE | 1.2.840.10008.5.1.4.1.2.1.2 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCU | None |
| Study Root Query/Retrieve Model – MOVE | 1.2.840.10008.5.1.4.1.2.2.2 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCU | None |

Table 23 Proposed Presentation Contexts - Move SCU "Import"

**Note:** C-MOVE extended negotiation is not supported by the SCU

#### 9.1.2.2.3 SOP Specific Conformance Statement - Move SCU "Import"

At association establishment time the C-MOVE presentation context shall be negotiated. The C-STORE sub-operations must be done on a different association to transfer images to the own Storage Service Class SCP.

The Move SCU interprets following status codes:

| Service Status | Meaning | Error Codes | Related Fields |
|---|---|---|---|
| Refused | Out of Resources - Unable to calculate number of matches | A701 | (0000,0902) |
| | Out of Resources - Unable to perform sub operations | A702 | (0000,1020)<br>(0000,1021)<br>(0000,1022)<br>(0000,1023) |
| Failed | Identifier does not match SOP Class | A900 | (0000,0901)<br>(0000,0902) |
| | Unable to process | CXXX | (0000,0901)<br>(0000,0902) |
| Cancel | Sub-operations terminated due to Cancel Indication | FE00 | (0000,1020)<br>(0000,1021)<br>(0000,1022) |

| | | | |
|---|---|---|---|
| | | | (0000,1023) |
| Warning | Sub-operations Complete - One or more Failures or Warnings | B000 | (0000,1020)<br>(0000,1021)<br>(0000,1022)<br>(0000,1023) |
| Success | Sub-operations Complete - No Failures or Warning | 0000 | (0000,1020)<br>(0000,1021)<br>(0000,1022)<br>(0000,1023) |
| Pending | Sub-operations are continuing | FF00 | (0000,1020)<br>(0000,1021)<br>(0000,1022)<br>(0000,1023) |

Table 24 Status Codes - Move SCU “Import”

### 9.1.3 Association Acceptance Policy

The Artis zee VC13 DICOM application will accept associations for the following DIMSE-C operations as SCP:

- C-FIND
- C-GET
- C-MOVE
- C-FIND-CANCEL
- C-GET-CANCEL
- C-MOVE-CANCEL

Extended negotiation - which is relational retrieve - is not supported for the above listed services. The Artis zee VC13 DICOM application does support multiple C-FIND requests over the same association, while multiple C-MOVE or C-GET operations are not supported over the same association.

#### 9.1.3.1 Real-World Activity - Find SCP

##### 9.1.3.1.1 Associated Real-World Activity - Find SCP

The associated Real-World activity is to respond query requests to an SCU with the query model Patient Root, Study Root and Patient/Study Only. Relational retrieve operation is not supported. With a C-FIND-CANCEL request the running query can be canceled at any time.

Multiple C-FIND requests over the same association are supported.

##### 9.1.3.1.2 Accepted Presentation Contexts - Find SCP

The Artis zee VC13 DICOM application will accept Presentation Contexts as shown in the following table:

| Presentation Context Table | | | | | |
|---|---|---|---|---|---|
| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg. |
| Name | UID | Name List | UID List | | |
| Patient Root Query/Retrieve Model – FIND | 1.2.840.10008.5.1.4.1.2.1.1 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCP | None |

| Presentation Context Table | | | | | |
|---|---|---|---|---|---|
| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg. |
| Name | UID | Name List | UID List | | |
| Study Root Query/Retrieve Model – FIND | 1.2.840.10008.5.1.4.1.2.2.1 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCP | None |
| Patient/Study Only Query/Retrieve Model – FIND | 1.2.840.10008.5.1.4.1.2.3.1 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCP | None |

Table 25 Accepted Presentation Contexts - Find SCP

**Note:** C-FIND Extended Negotiation is not be supported.
The order of preference for accepting Transfer Syntaxes is: 1. Explicit VR Little Endian, 2. Explicit VR Big Endian, 3. Implicit VR Little Endian

#### 9.1.3.1.3 SOP Specific Conformance Statement - Find SCP

The Artis zee VC13 DICOM Query/Retrieve SCP supports hierarchical queries with all mandatory and optional search keys.

The query attribute contents will be treated case-sensitive.

With wildcard queries the symbol "?" is treated as "*" by the C-FIND SCP application. E.g. the query string of "?abc*" will be processed as "*abc*".

If the value for the patient-level unique key "Patient ID" is not known, it may be returned with zero length. The attribute "Image Comments" is not included in the C-FIND-RSP, if it is not set in the DB, even if it was requested as return key in the related C-FIND-RQ.

Usage of Storage Media File-Set ID, Retrieve AE Title with C-FIND-RSP message:

- The Storage Media File-Set ID - if existent - can be returned at Study/Series/Image Level. Only on Image Level, the values of ONLINE, NEARLINE of OFFLINE are returned to indicate the Storage Location of the related Instance.
- The Retrieve AE Title - if existent - can only be returned at Image Level (for Patient Root and Study Root models) or Study Level (for Patient/Study Only model).

Relational Queries are **not** supported.

A remote DICOM AE can cancel the running query by sending a C-FIND-CANCEL. Matches are possibly continuing (more C-FIND response with status PENDING) until the cancel operation has completed.

The supported attributes on the various query levels of the three supported information models are list in the tables of the following sections.

##### 9.1.3.1.3.1 Patient Root Information Model

| Attribute Name | Tag | Usage SCU | Matching |
|---|---|---|---|
| **Patient Level** | | | |
| Patient Name | (0010,0010) | R | single value, wildcard, universal |
| Patient ID | (0010,0020) | U | single value, wildcard, universal |
| Patient's Birth Date | (0010,0030) | O | single value, range, universal |
| Patient's Birth Time | (0010,0032) | O | single value, range, universal |
| Patient's Sex | (0010,0040) | O | single value, wildcard, universal |
| Ethnic Group | (0010,2160) | O | single value, wildcard, universal |
| Patient Comments | (0010,4000) | O | wildcard, universal |
| Number of Patient related Studies | (0020,1200) | O | universal |
| Number of Patient related Series | (0020,1202) | O | universal |
| Number of Patient related Instances | (0020,1204) | O | universal |
| **Study Level** | | | |
| Study Instance UID | (0020,000D) | U | single value, list of UIDs |
| Study ID | (0020,0010) | R | single value, wildcard, universal |
| Study Date | (0008,0020) | R | single value, range, universal |
| Study Time | (0008,0030) | R | single value, range, universal |
| Accession Number | (0008,0050) | R | single value, wildcard, universal |
| Referring Physician's Name | (0008,0090) | O | single value, wildcard, universal |

| Attribute Name | Tag | Usage SCU | Matching |
|---|---|---|---|
| Study Description | (0008,1030) | O | single value, wildcard, universal |
| Admitting Diagnoses Description | (0008,1080) | O | single value, wildcard, universal |
| Patient's Age | (0010,1010) | O | single value, wildcard, universal |
| Patient's Size | (0010,1020) | O | single value, universal |
| Patient's Weight | (0010,1030) | O | single value, universal |
| Occupation | (0010,2180) | O | single value, wildcard, universal |
| Additional Patient History | (0010,21B0) | O | wildcard, universal |
| Name of Physician reading Study | (0008,1060) | O | single value, wildcard, universal |
| Modalities in Study | (0008,0061) | O | multiple values, universal |
| Number of Study related Series | (0020,1206) | O | universal |
| Number of Study related Instances | (0020,1208) | O | universal |
| **Series Level** | | | |
| Series Instance UID | (0020,000E) | U | single value, list of UID |
| Series Number | (0020,0011) | R | single value, universal |
| Modality | (0008,0060) | R | single value, wildcard, universal |
| Laterality | (0020,0060) | O | single value, wildcard, universal |
| Body Part Examined | (0018,0015) | O | single value, wildcard, universal |
| Patient Position | (0018,5100) | O | single value, wildcard, universal |
| Smallest Pixel Value in Series | (0028,0108) | O | single value, universal |
| Largest Pixel Value in Series | (0028,0109) | O | single value, universal |
| Protocol Name | (0018,1030) | O | single value, wildcard, universal |
| Series Date | (0008,0021) | O | single value, range, universal |
| Series Time | (0008,0031) | O | single value, range, universal |
| Series Description | (0008,103E) | O | single value, wildcard, universal |
| Operators Name | (0008,1070) | O | single value, wildcard, universal |
| Performing Physician's Name | (0008,1050) | O | single value, wildcard, universal |
| Perf. Procedure Step Start Date | (0040,0244) | O | universal |
| Perf. Procedure Step Start Time | (0040,0245) | O | universal |
| Number of Series related Instances | (0020,1209) | O | universal |
| **Image Level** | | | |
| SOP Instance UID | (0008,0018) | U | single value, list of UID |
| Image Number | (0020,0013) | R | single value, universal |
| Image Date | (0008,0023) | O | single value, range, universal |
| Image Time | (0008,0033) | O | single value, range, universal |
| Modality | (0008,0060) | O | single value, wildcard, universal |
| Image Comments | (0020,4000) | O | Universal |

Table 26 Supported Query attributes sorted by Query Level – Patient Root Information Model

### 9.1.3.1.3.2 Study Root Information Model

| Attribute Name | Tag | Usage SCU | Matching |
|---|---|---|---|
| **Study Level** | | | |
| Patient Name | (0010,0010) | R | Single value, Wildcard, universal |
| Patient ID | (0010,0020) | R | Single Value, Wildcard, universal |
| Patient's Birth Date | (0010,0030) | O | Single Value, Range, universal |
| Patient's Birth Time | (0010,0032) | O | Single Value, Range, universal |
| Patient's Sex | (0010,0040) | O | Single Value, Wildcard, universal |
| Patient Comments | (0010,4000) | O | Wildcard, universal |
| Number of Patient related Studies | (0020,1200) | O | universal |
| Number of Patient related Series | (0020,1202) | O | universal |
| Number of Patient related Instances | (0020,1204) | O | universal |
| Study Instance UID | (0020,000D) | U | Single Value, List of UIDs |
| Study ID | (0020,0010) | R | Single Value, Wildcard, universal |
| Study Date | (0008,0020) | R | Single Value, Range, universal |
| Study Time | (0008,0030) | R | Single Value, Range, universal |
| Accession Number | (0008,0050) | R | Single Value, Wildcard, universal |
| Referring Physician's Name | (0008,0090) | O | Single Value, Wildcard, universal |
| Study Description | (0008,1030) | O | Single Value, Wildcard, universal |
| Admitting Diagnosis Description | (0008,1080) | O | Single Value, Wildcard, universal |
| Patient's Age | (0010,1010) | O | Single Value, Wildcard, universal |
| Patient's Size | (0010,1020) | O | Single Value, universal |
| Patient's Weight | (0010,1030) | O | Single Value, universal |
| Occupation | (0010,2180) | O | Single Value, Wildcard, universal |
| Additional Patient History | (0010,21B0) | O | Wildcard, universal |
| Name of Physician reading the Study | (0008,1060) | O | Single Value, Wildcard, universal |
| Modalities in Study | (0008,0061) | O | Multiple values, universal |
| Number of Study Related Series | (0020,1206) | O | universal |
| Number of Study Related Instances | (0020,1208) | O | universal |
| **Series Level** | | | |
| Series Instance UID | (0020,000E) | U | Single Value, List of UIDs |
| Series Number | (0020,0011) | R | Single Value, universal |
| Modality | (0008,0060) | R | Single Value, Wildcard, universal |
| Laterality | (0020,0060) | O | Single Value, Wildcard, universal |
| Body Part Examined | (0018,0015) | O | Single Value, Wildcard, universal |
| Patient Position | (0018,5100) | O | Single Value, Wildcard, universal |
| Smallest Pixel Value in Series | (0028,0108) | O | Single Value, universal |
| Largest Pixel Value in Series | (0028,0109) | O | Single Value, universal |
| Protocol Name | (0018,1030) | O | Single Value, Wildcard, universal |
| Series Date | (0008,0021) | O | Single Value, Range, universal |
| Series Time | (0008,0031) | O | Single Value, Range, universal |
| Series Description | (0008,103E) | O | Single Value, Wildcard, universal |
| Operator's Name | (0008,1070) | O | Single Value, Wildcard, universal |
| Performing Physician's Name | (0008,1050) | O | Single Value, Wildcard, universal |
| Performed Procedure Step Start Date | (0040,0244) | O | universal |
| Performed Procedure Step Start Time | (0040,0245) | O | universal |
| Number of Series related Instances | (0020,1209) | O | universal |
| **Image Level** | | | |
| SOP Instance UID | (0008,0018) | U | Single Value, List of UIDs |
| Image Number | (0020,0013) | R | Single Value, universal |
| Image Date | (0008,0023) | O | Single Value, Range, universal |
| Image Time | (0008,0033) | O | Single Value, Range, universal |
| Modality | (0008,0060) | O | Single Value, Wildcard, universal |

| Attribute Name | Tag | Usage SCU | Matching |
|---|---|---|---|
| Image Comments | (0020,4000) | O | universal |

Table 27 Supported Query attributes sorted by Query Level – Study Root Information Model

#### 9.1.3.1.3.3 Patient/Study Only Information Model

| Attribute Name | Tag | Usage SCU | Matching |
|---|---|---|---|
| **Patient Level** | | | |
| Patient Name | (0010,0010) | R | Single value, Wildcard, universal |
| Patient ID | (0010,0020) | U | Single Value, Wildcard, universal |
| Patient's Birth Date | (0010,0030) | O | Single Value, Range, universal |
| Patient's Birth Time | (0010,0032) | O | Single Value, Range, universal |
| Patient's Sex | (0010,0040) | O | Single Value, Wildcard, universal |
| Ethnic Group | (0010,2160) | O | Single Value, Wildcard, universal |
| Patient Comments | (0010,4000) | O | Wildcard, universal |
| Number of Patient related Studies | (0020,1200) | O | universal |
| Number of Patient related Series | (0020,1202) | O | universal |
| Number of Patient related Instances | (0020,1204) | O | universal |
| **Study Level** | | | |
| Study Instance UID | (0020,000D) | U | Single Value, List of UIDs |
| Study ID | (0020,0010) | R | Single Value, Wildcard, universal |
| Study Date | (0008,0020) | R | Single Value, Range, universal |
| Study Time | (0008,0030) | R | Single Value, Range, universal |
| Accession Number | (0008,0050) | R | Single Value, Wildcard, universal |
| Referring Physician's Name | (0008,0090) | O | Single Value, Wildcard, universal |
| Study Description | (0008,1030) | O | Single Value, Wildcard, universal |
| Admitting Diagnosis Description | (0008,1080) | O | Single Value, Wildcard, universal |
| Patient's Age | (0010,1010) | O | Single Value, Wildcard, universal |
| Patient's Size | (0010,1020) | O | Single Value, universal |
| Patient's Weight | (0010,1030) | O | Single Value, universal |
| Occupation | (0010,2180) | O | Single Value, Wildcard, universal |
| Additional Patient History | (0010,21B0) | O | Wildcard, universal |
| Name of Physician reading the Study | (0008,1060) | O | Single Value, Wildcard, universal |
| Modalities in Study | (0008,0061) | O | Multiple values, universal |
| Number of Study Related Series | (0020,1206) | O | universal |
| Number of Study Related Instances | (0020,1208) | O | universal |

Table 28 Supported Query attributes sorted by Query Level – Patient/Study only Information Model

The Find SCP returns following status codes:

| Service Status | Meaning | Error Codes | Related Fields |
|---|---|---|---|
| Refused | Out of Resources | A700 | (0000,0902) |
| Failed | Identifier does not match SOP Class | A900 | (0000,0901) (0000,0902) |
| | Unable to process | C001 | (0000,0901) (0000,0902) |
| Cancel | Matching terminated due to Cancel request | FE00 | None |
| Success | Matching is complete - No final Identifier is supplied | 0000 | None |
| Pending | Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys | FF00 | Identifier |
| | Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this identifier | FF01 | Identifier |

Table 29 Status Codes

### 9.1.3.2 Real-World Activity - Get SCP

#### 9.1.3.2.1 Associated Real-World Activity - Get SCP

The associated Real-World activity is to respond to retrieve requests initiated from a foreign SCU. The SCP supports the query model Patient Root, Study Root and Patient/Study Only. The Storage Service Class Conformance Statement describes the C-STORE service, which is generated by the C-GET service. Relational retrieve operation is not supported.

Multiple C-GET requests over the same association are not supported.

#### 9.1.3.2.2 Accepted Presentation Contexts - Get SCP

The Artis zee VC13 DICOM application will accept Presentation Contexts as shown in the following table:

| Presentation Context Table | | | | | |
|---|---|---|---|---|---|
| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg. |
| Name | UID | Name List | UID List | | |
| Patient Root Query/Retrieve Model – GET | 1.2.840.10008.5.1.4.1.2.1.3 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCP | None |
| Study Root Query/Retrieve Model – GET | 1.2.840.10008.5.1.4.1.2.2.3 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCP | None |
| Patient/Study Only Query/Retrieve Model – GET | 1.2.840.10008.5.1.4.1.2.3.3 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCP | None |

Table 30 Accepted Presentation Contexts - Get SCP

**Note:** C-GET Extended negotiation is not supported.
The order of preference for accepting Transfer Syntaxes is: 1. Explicit VR Little Endian, 2. Explicit VR Big Endian, 3. Implicit VR Little Endian.

#### 9.1.3.2.3 SOP Specific Conformance Statement - Get SCP

At association establishment time the C-GET presentation context must be negotiated along with the C-STORE sub-operations which must be accomplished on the same association as the C-GET operation. Relational retrieve operation is not supported.

The Get SCP returns following status codes:

| Service Status | Meaning | Error Codes | Related Fields |
|---|---|---|---|
| Refused | Out of Resources - Unable to calculate number of matches | A701 | (0000,0902) |
| | Out of Resources - Unable to perform sub operations | A702 | (0000,1020)<br>(0000,1021)<br>(0000,1022)<br>(0000,1023) |
| Failed | Identifier does not match SOP Class | A900 | (0000,0901)<br>(0000,0902) |
| | Unable to process | C001 | (0000,0901)<br>(0000,0902) |
| Cancel | Sub-operations terminated due to Cancel Indication | FE00 | (0000,1020)<br>(0000,1021)<br>(0000,1022)<br>(0000,1023) |
| Warning | Sub-operations Complete - One or more Failures of | B000 | (0000,1020) |

| Service Status | Meaning | Error Codes | Related Fields |
|---|---|---|---|
| | Warnings | | (0000,1021)<br>(0000,1022)<br>(0000,1023) |
| Success | Sub-operations Complete - No Failures or Warning | 0000 | (0000,1020)<br>(0000,1021)<br>(0000,1022)<br>(0000,1023) |
| Pending | Sub-operations are continuing | FF00 | (0000,1020)<br>(0000,1021)<br>(0000,1022)<br>(0000,1023) |

Table 31 Status Codes

### 9.1.3.3 Real-World Activity - Move SCP

#### 9.1.3.3.1 Associated Real-World Activity - Move SCP

The associated Real-World activity is to respond to retrieve requests to an SCU. The SCP supports the query model Patient Root, Study Root and Patient/Study Only. The Storage Service Class Conformance Statement describes the C-STORE service, which is generated by the C-MOVE service. Relational retrieve operation is not supported.

Multiple C-MOVE requests over the same association are not supported.

#### 9.1.3.3.2 Accepted Presentation Contexts - Move SCP

The Artis zee VC13 DICOM application will accept Presentation Contexts as shown in the following table:

| Presentation Context Table | | | | | |
|---|---|---|---|---|---|
| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg. |
| Name | UID | Name List | UID List | | |
| Patient Root Query/Retrieve Model – MOVE | 1.2.840.10008.5.1.4.1.2.1.2 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCP | None |
| Study Root Query/Retrieve Model – MOVE | 1.2.840.10008.5.1.4.1.2.2.2 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCP | None |
| Patient/Study Only Query/Retrieve Model – MOVE | 1.2.840.10008.5.1.4.1.2.3.2 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCP | None |

Table 32 Accepted Presentation Contexts - Move SCP

**Note:** C-MOVE Extended negotiation is not supported.
The order of preference for accepting Transfer Syntaxes is: 1. Explicit VR Little Endian, 2. Explicit VR Big Endian, 3. Implicit VR Little Endian.

#### 9.1.3.3.3 SOP Specific Conformance Statement - Move SCP

At association establishment time the C-MOVE presentation context shall be negotiated. The C-STORE sub-operations is done on a different association, specified in the C-MOVE request, to transfer images to a remote SCP of the Storage Service Class. Relational retrieve operation is not supported.

The Move SCP returns following status codes:

| Service Status | Meaning | Error Codes | Related Fields |
|---|---|---|---|
| Refused | Out of Resources - Unable to calculate number of matches | A701 | (0000,0902) |
| | Out of Resources - Unable to perform sub operations | A702 | (0000,1020)<br>(0000,1021)<br>(0000,1022)<br>(0000,1023) |
| Failed | Identifier does not match SOP Class | A900 | (0000,0901)<br>(0000,0902) |
| | Unable to process | C001 | (0000,0901)<br>(0000,0902) |
| Cancel | Sub-operations terminated due to Cancel Indication | FE00 | (0000,1020)<br>(0000,1021)<br>(0000,1022)<br>(0000,1023) |
| Warning | Sub-operations Complete - One or more Failures of Warnings | B000 | (0000,1020)<br>(0000,1021)<br>(0000,1022)<br>(0000,1023) |
| Success | Sub-operations Complete - No Failures or Warning | 0000 | (0000,1020)<br>(0000,1021)<br>(0000,1022)<br>(0000,1023) |
| Pending | Sub-operations are continuing | FF00 | (0000,1020)<br>(0000,1021)<br>(0000,1022)<br>(0000,1023) |

Table 33 Status Codes

# 10 Implementation Model Print

The Print Management Service Classes define an application-level class of services, which facilitate the printing of images on a hardcopy medium. The print management SCU and print management SCP are peer DICOM print management application entities. The Artis zee VC13 DICOM print application supports the print management DIMSE services to act as SCU.

## 10.1 Application Data Flow Diagram

The Artis zee VC13 DICOM network implementation acts as SCU for the print management network service. The product target Operating System is Windows XP.

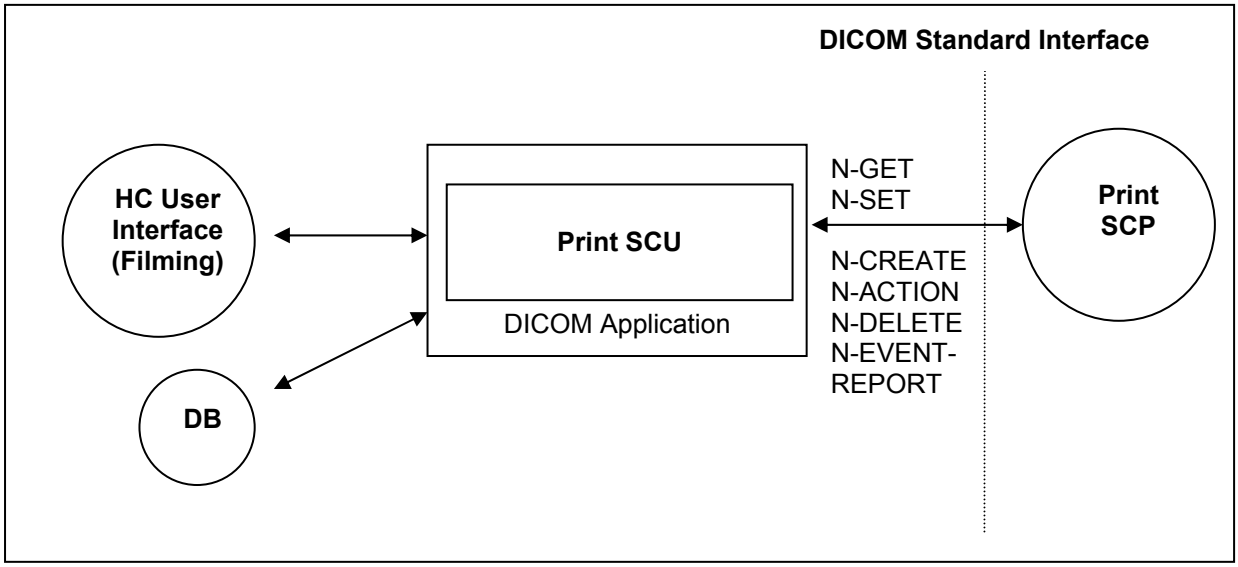


Figure 6 DICOM Application Data Flow Diagram – Print SCU

## 10.2 Functional Definition of Application Entities

The Print SCU is invoked by the user interface to setup film-sheet layout and whenever an image is ready to be printed on film. The Print SCU will hold and maintain all data needed to compile a complete film-sheet from the data (images, layout, configuration) received. Whenever a film-sheet is ready to print the related data is used to supply the Information to the SOP Classes of the Print Management Service Class. A queue is maintained, in order to intermediately store several film-sheets in case of resource problems on printer. The SCU will only supply and require the mandatory SOP Classes of the Print Management Service Class.

## 10.3 Sequencing of Real-World Activities

Not applicable

# 11 Application Entity Specification Print

## 11.1 Print Management AE Specification

The *syngo* print management SCU invokes print management DIMSE services to transfer images from the local AE to the remote SCP AE to print images with defined layout on a selected network-based DICOM hardcopy printer. This is done in a “full-page” print mode.

SIEMENS *syngo* DICOM products provide Standard Conformance to the following DICOM Print Management Meta SOP Classes as an SCU:

| SOP Class Name | SOP Class UID |
|---|---|
| Basic Grayscale Print Management Meta SOP Class | 1.2.840.10008.5.1.1.9 |
| - Basic Film Session SOP Class | 1.2.840.10008.5.1.1.1 |
| - Basic Film Box SOP Class | 1.2.840.10008.5.1.1.2 |
| - Basic Grayscale Image Box SOP Class | 1.2.840.10008.5.1.1.4 |
| - Printer SOP Class | 1.2.840.10008.5.1.1.16 |
| Print Job SOP Class | 1.2.840.10008.5.1.1.14 |

Table 34 Basic Grayscale Print Management Meta SOP Class

### 11.1.1 Association Establishment Policies

#### 11.1.1.1 General

Whenever a film is completely set up and printed by command or automatism, the job is prepared for processing. As soon as the queue is ready to process, the job is activated and works according to the processing data. The related Print application will initiate an association to the print destination and process the printing of the related information.

The default PDU size used will be 256 KB.

#### 11.1.1.2 Number of Associations

The *syngo* DICOM Print application initiates one association at a time for each different print device configured.

#### 11.1.1.3 Asynchronous Nature

The *syngo* DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

#### 11.1.1.4 Implementation Identifying Information

| | |
|---|---|
| Implementation Class UID | 1.3.12.2.1107.5.9.20000101 |
| Implementation Version Name | SIEMENS_SWFSYNGO |

Table 35 Implementation Identifying Information

### 11.1.2 Association Initiation Policy

Triggered by the Print job queue the Print Management SCU establishes an association by using the DICOM association services. With the help of the N-GET request for the Printer SOP Class the Status is determined before printing.

With no problem encountered with the N-CREATE/N-SET Services for the related Basic Print SOP Classes the film sheet is set up for printing and the image(s) is(are) transferred to the printer device.

After the last film is printed from queue, the Print application will leave open the association for another 60 seconds. If a new film job is ready for printing within this time-limit, the job will be immediately processed over the still open association. If there is no new job, the association is closed if the time-out elapsed. This is done to optimize automated printing.

During the “idle-time” (no open association to printer) the Print application will issue a cyclic camera status request (using N-GET of Printer SOP Class) every 5 minutes.

#### 11.1.2.1 Associated Real-World Activity

#### 11.1.2.1.1 Associated Real-World Activity – Printing a Printer Job Queue Entry

Whenever the user prepares a film-sheet it is forwarded to the Printer Job queue. If the associated Printer device is available, the job is activated by opening an association to this device.

The film sheet is internally processed, converted to a Standard/1-1 page and then the page image is sent.

If the response from the remote application contains a status other than Success or Warning the association is aborted.

#### 11.1.2.1.2 Proposed Presentation Context (Presentation Context Table)

The Siemens *syngo* DICOM Print application will propose Presentation Contexts as shown in the following table:

| Presentation Context Table | | | | | |
|---|---|---|---|---|---|
| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg. |
| Name | UID | Name List | UID List | | |
| Basic Grayscale Print Management Meta SOP class | 1.2.840.10008.5.1.1.9 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCU | None |
| Basic film session SOP class | 1.2.840.10008.5.1.1.1 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCU | None |
| Basic Film Box SOP class | 1.2.840.10008.5.1.1.2 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCU | None |
| Basic Grayscale Image Box SOP class | 1.2.840.10008.5.1.1.4 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCU | None |
| Printer SOP class | 1.2.840.10008.5.1.1.16 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCU | None |
| Print Job SOP class | 1.2.840.10008.5.1.1.14 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCU | None |

Table 36 Proposed Presentation Contexts

### 11.1.2.1.3 SOP specific Conformance Statement – Meta SOP Classes

The *syngo* DICOM print management SCU conforms to the DICOM Basic Grayscale Print Management Meta SOP.

The application uses a configuration platform to define the properties of the connected DICOM SCP, e.g.:

- maximum number of print jobs in the queue
- maximum number of print copies
- supported film sizes of the connected DICOM SCP
- supported film formats of the DICOM SCP
- lookup table definition.

The printing is only suspended in the case of a failure return status of the SCP.

#### 11.1.2.1.3.1 Basic Film Session SOP class

The Basic Film Session information object definition describes all the user-defined parameters, which are common for all the films of a film session. The Basic Film Session refers to one or more Basic Film Boxes, that are printed on one hardcopy printer.

The *syngo* DICOM print management SCU supports the following DIMSE Service elements for the Basic Film Session SOP Class as SCU:

- N-CREATE
- N-DELETE

The Basic Film Session SOP Class N-CREATE-RQ (SCU) uses the following attributes:

| Attribute Name | Tag | Usage SCU | Supported Values |
|---|---|---|---|
| Number of Copies | (2000,0010) | U | 1 |
| Medium Type | (2000,0030) | U | BLUE FILM<br>CLEAR FILM<br>PAPER |
| Film Destination | (2000,0040) | U | MAGAZINE<br>PROCESSOR |

Table 37 Used Basic Film Session N-CREATE-RQ attributes

The number of Copies sent to the DICOM Printer is always 1, the job is sent n times for n copies.

The affected SOP Instance UID received with N-CREATE-RSP message will be kept internally and used for later requests (e.g. N-DELETE-RQ) on the Basic Film Session – see below:

| Attribute Name | Tag | Source of Information |
|---|---|---|
| Requested SOP Instance UID | (0000,1000)<br>→ (0000,1001) | Affected SOP Instance UID of N-CREATE-RSP on Basic Film Session |

Table 38 Attributes of N-DELETE-RQ on Basic Film Session SOP Class

The N-DELETE-RQ on the Basic Film Session SOP Class is used to remove the complete Basic Film Session SOP Instance hierarchy.

The Basic Film Session SOP class interprets the following status codes (from N-CREATE-RSP, N-DELETE-RSP messages):

| Service Status | Meaning | Error Codes |
|---|---|---|
| Failed | Film session SOP instances hierarchy does not contain film box SOP instances | C600 |
| | Unable to create print job, print queue is full | C601 |
| | Image size is larger than images box size | C603 |
| Warning | Memory allocation not supported | B600 |
| | Film session printing is not supported | B601 |
| | Film box does not contain image box (empty page) | B602 |
| Success | Film belonging to the film session are accepted for printing | 0000 |

Table 39 Basic Film Session SOP Status

### 11.1.2.1.3.2 Basic Film Box SOP class

The Basic Film Box information object definition describes all the user-defined parameters of one film of the film session. The Basic Film Box information description defines the presentation parameters, which are common for all images on a given sheet of film.

The Basic Film Box refers to one or more Image Boxes.

Supported Service Elements as SCU are:

- N-CREATE
- N-ACTION
- N-DELETE

The Basic Film Box SOP class N-CREATE-RQ message uses the following attributes (the actual values for each attribute depend on DICOM printer configuration within the *syngo* DICOM print management SCU):

| Attribute Name | Tag | Usage SCU | Supported Values |
|---|---|---|---|
| Image Display Format | (2010,0010) | M | STANDARD\1,1 |
| Referenced Film Session Sequence | (2010,0500) | M | |
| > Referenced SOP Class UID | (0008,1150) | M | 1.2.840.10008.5.1.1.1 |
| > Referenced SOP Instance UID | (0008,1155) | M | |
| Film Orientation | (2010,0040) | M | PORTRAIT |
| Film Size ID | (2010,0050) | M | 8INX10IN, 10INX12IN, 10INX14IN, 11INX14IN,, 14INX14IN, 14INX17IN, 24CMX24CM, 24CMX30CM |
| Magnification Type | (2010,0060) | M | BILINEAR, CUBIC, NONE, REPLICATE |
| Border Density | (2010,0100) | U | BLACK, WHITE |
| Max Density | (2010,0130) | U | 0 < Value |
| Min Density | (2010,0120) | U | 0 < Value < 50 |
| Illumination | (2010,015E) | U | 0 < Value Required if Presentation LUT is present. |
| Reflective Ambient Light | (2010,0160) | U | 0 < Value Required if Presentation LUT is present. |
| Referenced Presentation LUT Sequence | (2050,0500) | U | |

Table 40 Used Film Box N-CREATE-RQ attributes

The N-CREATE-RSP message from the Print SCP includes the Referenced Image Box Sequence with SOP Class/Instance UID pairs which will be kept internally to be further used for the subsequent Basic Image Box SOP Class N-SET-RQ messages.

When all Image Boxes (including parameters) for the film-sheet have been set, the *syngo* DICOM print manager will issue a N-ACTION-RQ message with the SOP Instance UID of the Basic Film Box and the Action Type ID of 1.

The affected SOP Instance UID received with N-CREATE-RSP message will be kept internally and used for later requests (e.g. N-DELETE-RQ) on the Basic Film Box - see below:

| Attribute Name | Tag | Source of Information |
|---|---|---|
| Requested SOP Instance UID | (0000,1000) → (0000,1001) | Affected SOP Instance UID of N-CREATE-RSP on Basic Film Box |

Table 41 Attributes of N-DELETE-RQ on Basic Film Session SOP Class

The Basic Film Box SOP class interprets the following status codes:

| Service Status | Meaning | Error Codes |
|---|---|---|
| Failure | Unable to create print job, print queue is full | C602 |
| | Image size is larger than images box size | C603 |
| Warning | Film box does not contain image box (empty page) | B603 |
| | Requested MinDensity or MaxDensity outside of Printer's operating range | B605 |
| Success | Film accepted for printing | 0000 |

Table 42 Basic Film Session SOP Status

### 11.1.2.1.3.3 Basic Grayscale Image Box SOP Class

The Basic Grayscale Image Box information object definition is the presentation of an image and image related data in the image area of a film. The Basic Image Box information describes the presentation parameters and image pixel data, which apply to a single image of a sheet of film.

The Grayscale Image Box SOP Class uses only the N-SET-RQ with the following attributes:

| Attribute Name | Tag | Usage SCU | Supported Values |
|---|---|---|---|
| Image Position | (2020,0010) | M | 1 |
| BASIC Grayscale Image Sequence | (2020,0110) | M | |
| > Samples per Pixel | (0028,0002) | M | 1 |
| > Photometric Interpretation | (0028,0004) | M | MONOCHROME2 |
| > Rows | (0028,0010) | M | |
| > Columns | (0028,0011) | M | |
| > Pixel Aspect Ratio | (0028,0034) | M | |
| > Bits Allocated | (0028,0100) | M | 8 or 16 |
| > Bits Stored | (0028,0101) | M | 8 or 12 |
| > High Bit | (0028,0102) | M | 7 or 11 |
| > Pixel Representation | (0028,0103) | M | 0 |
| > Pixel Data | (7FE0,0010) | M | |

Table 43 Mandatory Basic Grayscale Image Box N-SET attributes

The Grayscale Image Box SOP class interpret the following status codes:

| Service Status | Meaning | Error Codes |
|---|---|---|
| Failure | Image contains more pixel than printer can print in Image Box | C603 |
| | Insufficient memory in printer to store the image | C605 |
| Warning | Requested MinDensity or MaxDensity outside of Printer's operating range | B605 |
| Success | | 0000 |

Table 44 Basic Grayscale Image Box SOP Status

### 11.1.2.1.3.4 Printer SOP Class

The Printer SOP Class is the possibility to monitor the status of the hardcopy printer in a synchronous and an asynchronous way.

The SCU uses the mandatory N-EVENT Report DIMSE service to monitor the changes of the printer status in an asynchronous way.

It can directly ask the Printer (SCP) for its status or receive Events from the Printer asynchronously:

- N-GET as SCU
- N-EVENT-REPORT as SCU In both cases the following information is supported:

Used Printer N-EVENT Report attributes

| Event-type Name | Event | Attributes | Tag | Usage SCU |
|---|---|---|---|---|
| Normal | 1 | | | |
| Warning | 2 | Printer Status Info | (2110,0020) | U |
| Failure | 3 | Printer Status Info | (2110,0020) | U |

Table 45 Used Printer N-EVENT report attributes

#### 11.1.2.1.3.4.1.1.1 Mandatory Printer N-GET-RSP, N-EVENT-REPORT-RQ attributes

| Attribute Name | Tag | Usage SCP | Supported Values |
|---|---|---|---|
| Printer Status | (2110,0010) | M | NORMAL, FAILURE, WARNING |
| Printer Status Info | (2110,0020) | M | See tables in Annex for details. |

Table 46 Mandatory Printer N-GET-RSP, N-EVENT-RQ attributes

**Note:** For a detailed description on how *syngo* reacts on different printer status messages, please refer to the Annex section "DICOM Print SCU – detailed status displays".

#### 11.1.2.1.3.5 Print Job SOP Class

The Print Job SOP Class is the possibility to monitor the execution of the print process.

The *syngo* DICOM Print Management application supports the optional N-EVENT-REPORT DIMSE Service to receive the changes of the Print Job Status in an asynchronous way.

It can receive Events from the Print SCP asynchronously

Note: syngo does not support receiving N-EVENT-REPORT from camera during print sessions, normally this is configurable in the camera.

N-EVENT-REPORT The following information is supported:

| Event-type Name | Event | Attributes | Tag | Usage SCU |
|---|---|---|---|---|
| Normal | 1 | Execution Status Info | (2100,0030) | U |
| | | Print Job ID | (2100,0010) | -- (Print Queue Management SOP Class not supported) |
| | | Film Session Label | (2000,0050) | U |
| | | Printer Name | (2110,0030) | U |
| Printing | 2 | Execution Status Info | (2100,0030) | U |
| | | Print Job ID | (2100,0010) | -- (Print Queue Management SOP Class not supported) |
| | | Film Session Label | (2000,0050) | U |
| | | Printer Name | (2110,0030) | U |
| Done | 3 | Execution Status Info | (2100,0030) | U |
| | | Print Job ID | (2100,0010) | -- (Print Queue Management SOP Class not supported) |
| | | Film Session Label | (2000,0050) | U |
| | | Printer Name | (2110,0030) | U |
| Failure | 4 | Execution Status Info | (2100,0030) | U |
| | | Print Job ID | (2100,0010) | -- (Print Queue Management SOP Class not supported) |
| | | Film Session Label | (2000,0050) | U |
| | | Printer Name | (2110,0030) | U |

Table 47 Used Print Job N-EVENT-REPORT attributes

**Note:** For a detailed description on how *syngo* reacts on different printer status messages, please refer to the Annex section “DICOM Print SCU – detailed status displays”.

### 11.1.3 Association Acceptance Policy

Not applicable

# 12 Implementation Model Worklist

The Basic Worklist Management Service class defines an application-level class of service that facilitates the transfer of worklists from the information system to the imaging modality. The worklist is queried by the AE and supplies the SCU with the scheduled tasks, which have to be performed on the modality. The Artis zee VC13 DICOM worklist application supports the worklist service as SCU.

## 12.1 Application Data Flow Diagram

The Artis zee VC13 DICOM network implementation acts as SCU for the Basic Worklist Service using the Modality Worklist SOP Class. The product target Operating System is Windows XP.

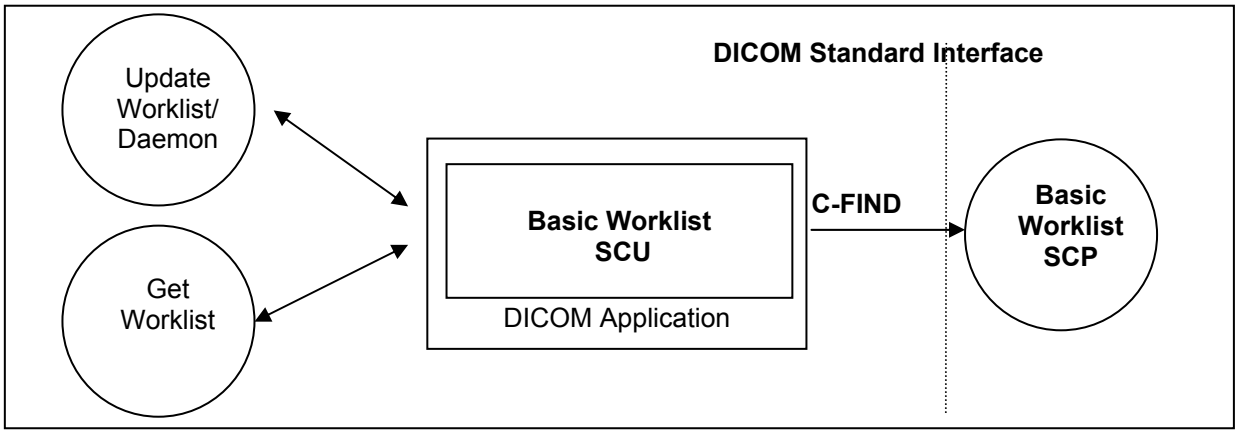


**Figure 7 Artis zee VC13 Application Flow Diagram – Basic Worklist SCU**

## 12.2 Functional Definitions of Application Entities

The worklist SCU (“broad query”) is invoked from the patient browser user interface or by timer to request the worklist from a remote Information System (Modality Worklist Class SCP). This is done to perform a match to the internal worklist query keys specified in the C-Find DIMSE service issued for the Modality Worklist Model.

The worklist SCP responses to the C-FIND query and scheduled imaging service requests (scheduled procedure steps) and patient demographic information will be downloaded from the information system to the Artis zee VC13 modality. All information retrieved will be held in the scheduling database for usage during Patient registration procedure.

Furthermore, the patient based Query dialog from the patient browser allows to enter specific matching criteria ("narrow query") for the worklist query. With the response data the Patient Registration dialog can be populated according availability within the worklist response identifier.

## 12.3 Sequencing of Real-World Activities

The “narrow” (interactive) Worklist Query requires that sufficient matching keys or a unique matching key are/is entered before the query is issued. Only then a single response can be expected to complete the registration dialog.

# 13 Application Entity Specification Worklist

## 13.1 Modality Worklist Service AE Specification

The Modality worklist SCU (patient registration in conjunction with the network application) requests that the remote SCP performs a match of all keys specified in the query against the information in its worklist database.

The Artis zee VC13 DICOM network implementation acts as SCU for the Basic Worklist Service using the Modality Worklist SOP Class:

| SOP Class Name | SOP Class UID |
|---|---|
| Modality Worklist Information Model - FIND | 1.2.840.10008.5.1.4.31 |

Table 48 SOP Classes as a SCU

### 13.1.1 Association Establishment Policies

#### 13.1.1.1 General

It is possible to configure a cyclic update of the modality scheduler database through a background worklist request with date/time and modality information.

In addition, the user can request worklist update with “Update Worklist”. No duplicate entries will be added in the Scheduler DB. Entries are uniquely identified by the Study Instance UID (0020,000D) for the Requested Procedure and the SPS ID (0040,009) in the SPS Sequence (0040,0100).

An interactive worklist query can be issued with search criteria entered in the patient based Query dialog from the patient browser.

The default PDU size used will be 256 KB.

#### 13.1.1.2 Number of Associations

The Artis zee VC13 DICOM application initiates one association at a time to query worklist entry data.

#### 13.1.1.3 Asynchronous Nature

The Artis zee VC13 DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

#### 13.1.1.4 Implementation Identifying Information

| | |
|---|---|
| Implementation Class UID | 1.3.12.2.1107.5.9.20000101 |
| Implementation Version Name | SIEMENS_SWFSYNGO |

Table 49 Implementation Identifying Information

### 13.1.2 Association Initiation Policy

The network application will cyclically query the worklist provider and by request from the patient registration interface. It establishes an association by using the DICOM association services. During association establishment the negotiation of SOP classes to exchange the capabilities of the SCU and the SCP is not supported.

The following DIMSE-C operation is supported as SCU:

- C-FIND

#### 13.1.2.1 Real-World Activity

##### 13.1.2.1.1 Associated Real-World Activity - Query (Update) Worklist

A network application will perform worklist queries with the C-FIND request at regular intervals. In addition it can be triggered by immediate request. The received worklist items will be compared with the contents of the local scheduler database. New items will be inserted into scheduler database.

After each broad-query, all RP/SPS that were canceled or rescheduled to another modality at the RIS will be automatically removed from the Scheduler DB if :

1. the Examination of this procedure has not been started or finished yet, and
2. the corresponding configuration item “Automatic removal of canceled/rescheduled Request” was checked in the Service UI under DICOM/HIS-RIS Node.

No automatic clean-up of the scheduler DB is performed after a Patient base Query since the worklist received does not give the complete list of all currently scheduled procedures for the modality.

##### 13.1.2.1.2 Proposed Presentation Contexts

The Artis zee VC13 DICOM application will propose Presentation Contexts as shown in the following table:

| Presentation Context Table | | | | | |
|---|---|---|---|---|---|
| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg. |
| Name | UID | Name List | UID List | | |
| Modality Worklist Information Model- FIND | 1.2.840.10008.5.1.4.31 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCU | None |

Table 50 Proposed Presentation Contexts

##### 13.1.2.1.3 SOP Specific Conformance Statement

- Search Key Attributes of the Worklist C-FIND

  The Artis zee VC13 DICOM worklist SCU supports “broad worklist queries” with all required search keys. The following tables describe the “broad query” search keys that the SCU supports.

| Attribute Name | Tag | Matching Key Type | Query Value |
|---|---|---|---|
| Scheduled Procedure Step | | | |
| Scheduled Procedure Step Sequence | (0040,0100) | R | |
| >Scheduled Station AE Title<br>*(This depends on user configuration (Options->Configuration->Patient Registration) if the "own AET" is provided or not. Use the "HIS/RIS" tab card for configuration.)* | (0040,0001) | R | <own AET> or <zero length> |
| >Scheduled Procedure Step Start Date<br>*(It depends on user configuration (Options->Configuration->Patient Registration) if the actual Date with a full time range or an interactive input dialog for date/time specification is used.)* | (0040,0002) | R | <act. Date>-<act. Date> or range from UI |
| >Scheduled Procedure Step Start Time<br>*(It depends on user configuration (Options->Configuration->Patient Registration) if the actual Date with a full time range or an interactive input dialog for date/time specification is used.)* | (0040,0003) | R | 00.00-235959.00 or range from UI |
| >Modality<br>*(This depends on user configuration (Options->Configuration->Patient Registration) if the "own Modality" is provided or not. Use the "HIS/RIS" tab card for configuration.)* | (0008,0060) | R | <zero length> or <own Modality> |
| >Scheduled Performing Physician | (0040,0006) | R | NULL |

Table 51 Supported Broad Worklist Query Search Key Attributes

- Return Key Attributes of the Worklist C-FIND

  The Artis zee VC13 DICOM worklist SCU supports worklist queries with return key attributes of all types. The following tables describe the return keys that the SCU supports.

  An “x” in the **UI** column will indicate the attribute is visualized when browsing the Worklist results with Patient Browser and/or during Patient Registration. The Patient Browser display is additionally influenced by the related Browser configuration.

  A tag in the **IOD** column will indicate that the related attribute is included into the SOP Instances of the IODs created during processing of this worklist request.

  A tag in the **MPPS** column will indicate that the related attribute is included into the SOP Instances of the MPPS objects created during processing of this worklist request. ( See also the tables “Attributes used for the Performed Procedure Step N-CREATE” and “Attributes used for the Performed Procedure Step N-SET”.)

| Attribute Name | Tag | Return Key Type | UI | IOD | MPPS |
|---|---|---|---|---|---|
| **SOP Common** | | | | | |
| Specific Character Set | (0008,0005) | 1C | - | (0008,0005) | (0008,0005) |
| **Scheduled Procedure Step** | | | | | |
| Scheduled Procedure Step Sequence | (0040,0100) | 1 | | | |
| >Modality | (0008,0060) | 1 | x | (0008,0060) | (0008,0060) |
| >Requested Contrast Agent | (0032,1070) | 2C | x | | |
| >Scheduled Station AE Title<br>*(“Scheduled Station AE Title” is taken as default for “Performed Station AE Title”)* | (0040,0001) | 1 | x | | (0040,0241) |
| >Scheduled Procedure Step Start Date | (0040,0002) | 1 | x | | |
| >Scheduled Procedure Step Start Time | (0040,0003) | 1 | x | | |
| >Scheduled Procedure Step End Date | (0040,0004) | 3 | - | | |
| >Scheduled Procedure Step End Time | (0040,0005) | 3 | - | | |

| Attribute Name | Tag | Return Key Type | UI | IOD | MPPS |
|---|---|---|---|---|---|
| >Scheduled Performing Physician's Name *("Scheduled Performing Physician's Name" is taken as default for "Performing Physician's Name")* | (0040,0006) | 1 | x | (0008,1050) | (0008,1050) |
| >Scheduled Procedure Step Description *("Scheduled Procedure Step Description" is taken as default for "Performed Procedure Step Description")* | (0040,0007) | 1C | x | (0040,0007) (0040,0254) | (0040,0007) (0040,0254) |
| >Scheduled Protocol Code Sequence *(universal Sequence Match) ("Scheduled Protocol Code Sequence" is taken as default for "Performed Protocol Code Sequence")* | (0040,0008) | 1C | - | (0040,0008) (0040,0260) | (0040,0008) (0040,0260) |
| >>Code Value | (0008,0100) | 1C | x | | |
| >>Coding Scheme Designator | (0008,0102) | 1C | x | | |
| >>Coding Scheme Version | (0008,0103) | 3 | x | | |
| >>Code Meaning | (0008,0104) | 3 | x | | |
| >Scheduled Procedure Step ID *("Scheduled Procedure Step ID" is taken as default for "Performed Procedure Step ID")* | (0040,0009) | 1 | x | (0040,0009) (0040,0253) | (0040,0009) (0040,0253) |
| >Scheduled Station Name | (0040,0010) | 2 | x | | |
| >Scheduled Procedure Step Location *("Scheduled Procedure Step Location" is taken as default for "Performed Location")* | (0040,0011) | 2 | x | | (0040,0243) |
| >Pre-Medication | (0040,0012) | 2C | x | | |
| >Scheduled Procedure Step Status | (0040,0020) | 3 | x | | |
| >Comments on the Scheduled Procedure Step | (0040,0400) | 3 | - | | |
| **Requested Procedure** | | | | | |
| Referenced Study Sequence *(universal Sequence Match)* | (0008,1110) | 2 | - | (0008,1110) | (0008,1110) |
| >Referenced SOP Class UID | (0008,1150) | 1C | - | | |
| >Referenced SOP Instance UID | (0008,1155) | 1C | - | | |
| Study Instance UID | (0020,000D) | 1 | - | (0020,000D) | (0020,000D) |
| Requested Procedure Description | (0032,1060) | 1C | x | (0032,1060) | (0032,1060) |
| Requested Procedure Code Sequence *(universal Sequence Match) ("Requested Procedure Code Sequence" is taken as default for "Procedure Code Sequence")* | (0032,1064) | 1C | - | (0008,1032) (0032,1064) | (0008,1032) |
| >Code Value | (0008,0100) | 1C | x | | |
| >Coding Scheme Designator | (0008,0102) | 1C | x | | |
| >Coding Scheme Version | (0008,0103) | 3 | x | | |
| >Code Meaning | (0008,0104) | 3 | x | | |
| Requested Procedure ID *("Requested Procedure ID" is taken as default for "Study ID")* | (0040,1001) | 1 | x | (0040,1001) (0020,0010) | (0040,1001) (0020,0010) |
| Reason for the Requested Procedure | (0040,1002) | 3 | - | | |
| Requested Procedure Priority | (0040,1003) | 2 | x | | |
| Patient Transport Arrangements | (0040,1004) | 2 | - | | |
| Requested Procedure Location | (0040,1005) | 3 | - | | |
| Confidentiality Code | (0040,1008) | 3 | - | | |
| Reporting Priority | (0040,1009) | 3 | - | | |
| Names of intended Recipients of Results | (0040,1010) | 3 | - | (0008,1048) | |
| Requested Procedure Comments | (0040,1400) | 3 | x | | |
| **Imaging Service Request** | | | | | |
| Accession Number | (0008,0050) | 2 | x | (0008,0050) | (0008,0050) |
| Referring Physician's Name | (0008,0090) | 2 | x | (0008,0090) | |
| Requesting Physician | (0032,1032) | 2 | x | (0032,1032) (0008,1048) | |
| Requesting Service | (0032,1033) | 3 | x | (0032,1033) | |
| Issuing Date of Imaging Service Request | (0040,2004) | 3 | - | | |
| Issuing Time of Imaging Service Request | (0040,2005) | 3 | - | | |
| Placer Order Number / Imaging Service Request | (0040,2016) | 3 | - | | (0040,2016) |

| Attribute Name | Tag | Return Key Type | UI | IOD | MPPS |
|---|---|---|---|---|---|
| *(Old tag (0040,2006) is retired and not used.)* | | | | | |
| Filler Order Number / Imaging Service Request *(Old tag (0040,2007) is retired and not used.)* | (0040,2017) | 3 | - | | (0040,2017) |
| Order entered by … | (0040,2008) | 3 | - | | |
| Order Enterer's location | (0040,2009) | 3 | - | | |
| Order Callback Phone Number | (0040,2010) | 3 | - | | |
| Imaging Service Request Comments | (0040,2400) | 3 | x | | |
| **Visit Identification** | | | | | |
| Institution Name | (0008,0080) | 3 | x | (0008,0080) | |
| Institution Address | (0008,0081) | 3 | - | | |
| Institution Code Sequence *(universal Sequence Match)* | (0008,0082) | 3 | - | | |
| >Code Value | (0008,0100) | 1C | - | | |
| >Coding Scheme Designator | (0008,0102) | 1C | - | | |
| >Coding Scheme Version | (0008,0103) | 3 | - | | |
| >Code Meaning | (0008,0104) | 3 | - | | |
| Admission ID | (0038,0010) | 2 | x | | |
| Issuer of Admission ID | (0038,0011) | 3 | - | | |
| **Visit Status** | | | | | |
| Visit Status ID | (0038,0008) | 3 | - | | |
| Current Patient Location | (0038,0300) | 2 | x | | |
| Patient's Institution Residence | (0038,0400) | 3 | - | | |
| Visit Comments | (0038,4000) | 3 | - | | |
| **Visit Relationship** | | | | | |
| Referenced Study Sequence *(universal Sequence Match)* | (0008,1110) | 3 | - | | |
| >Referenced SOP Class UID | (0008,1150) | 1C | - | | |
| >Referenced SOP Instance UID | (0008,1155) | 1C | - | | |
| Referenced Patient Sequence *(universal Sequence Match)* | (0008,1120) | 2 | - | | (0008,1120) |
| >Referenced SOP Class UID | (0008,1150) | 1C | - | | |
| >Referenced SOP Instance UID | (0008,1155) | 1C | - | | |
| **Visit Admission** | | | | | |
| Referring Physician's Name | (0008,0090) | 2 | x | (0008,0090) | |
| Admitting Diagnosis Description | (0008,1080) | 3 | x | (0008,1080) | |
| **Patient Identification** | | | | | |
| Patient's Name | (0010,0010) | 1 | x | (0010,0010) | (0010,0010) |
| Patient ID | (0010,0020) | 1 | x | (0010,0020) | (0010,0020) |
| Issuer of Patient ID | (0010,0021) | 3 | - | (0010,0021) | |
| Other Patient IDs | (0010,1000) | 3 | x | (0010,1000) | |
| Other Patient Names | (0010,1001) | 3 | x | (0010,1001) | |
| Patient's Birth Name | (0010,1005) | 3 | - | (0010,1005) | |
| Patient's Mother's Birth Name | (0010,1060) | 3 | - | (0010,1060) | |
| Medical Record Locator | (0010,1090) | 3 | - | (0010,1090) | |
| **Patient Demographic** | | | | | |
| Patient's Birth Date | (0010,0030) | 2 | x | (0010,0030) | (0010,0030) |
| Patient's Birth Time | (0010,0032) | 3 | - | (0010,0032) | |
| Patient's Sex | (0010,0040) | 2 | x | (0010,0040) | (0010,0040) |
| Patient's Insurance Plan Code Sequence *(universal Sequence Match)* | (0010,0050) | 3 | - | (0010,0050) | |
| >Code Value | (0008,0100) | 1C | - | | |
| >Coding Scheme Designator | (0008,0102) | 1C | - | | |
| >Coding Scheme Version | (0008,0103) | 3 | - | | |
| >Code Meaning | (0008,0104) | 3 | - | | |
| Patient's Age | (0010,1010) | 3 | x | (0010,1010) | |

| Attribute Name | Tag | Return Key Type | UI | IOD | MPPS |
|---|---|---|---|---|---|
| Patient's Size | (0010,1020) | 3 | x | (0010,1020) | |
| Patient's Weight | (0010,1030) | 2 | x | (0010,1030) | |
| Patient's Address | (0010,1040) | 3 | x | (0010,1040) | |
| Military Rank | (0010,1080) | 3 | x | (0010,1080) | |
| Branch of Service | (0010,1081) | 3 | - | (0010,1081) | |
| Country of Residence | (0010,2150) | 3 | - | (0010,2150) | |
| Region of Residence | (0010,2152) | 3 | - | (0010,2152) | |
| Patient's Telephone Numbers | (0010,2154) | 3 | - | (0010,2154) | |
| Ethnic Group | (0010,2160) | 3 | x | (0010,2160) | |
| Occupation | (0010,2180) | 3 | - | (0010,2180) | |
| Patient's Religious Preference | (0010,21F0) | 3 | - | (0010,21F0) | |
| Patient Comments | (0010,4000) | 3 | x | (0010,4000) | |
| Patient Data Confidentiality Constraint Description | (0040,3001) | 2 | x | (0040,3001) | |
| **Patient Medical** | | | | | |
| Medical Alerts | (0010,2000) | 2 | x | (0010,2000) | |
| Contrast Allergies | (0010,2110) | 2 | x | (0010,2110) | |
| Pregnancy Status | (0010,21C0) | 2 | x | (0010,21C0) | |
| Smoking Status | (0010,21A0) | 3 | x | (0010,21A0) | |
| Last Menstrual Date | (0010,21D0) | 3 | x | (0010,21D0) | |
| Additional Patient History | (0010,21B0) | 3 | x | (0010,21B0) | |
| Special Needs | (0038,0050) | 2 | x | (0038,0050) | |
| Patient State | (0038,0500) | 2 | x | (0038,0500) | |
| **Patient Relationship** | | | | | |
| Referenced Study Sequence *(universal Sequence Match)* | (0008,1110) | 3 | - | | |
| >Referenced SOP Class UID | (0008,1150) | 1C | - | | |
| >Referenced SOP Instance UID | (0008,1155) | 1C | - | | |
| Referenced Visit Sequence *(universal Sequence Match)* | (0008,1125) | 3 | - | | |
| >Referenced SOP Class UID | (0008,1150) | 1C | - | | |
| >Referenced SOP Instance UID | (0008,1155) | 1C | - | | |
| Referenced Patient Alias Sequence *(universal Sequence Match)* | (0038,0004) | 3 | - | | |
| >Referenced SOP Class UID | (0008,1150) | 1C | - | | |
| >Referenced SOP Instance UID | (0008,1155) | 1C | - | | |

Table 52 Basic Worklist C-FIND-RSP Return Key Attributes

### 13.1.2.1.4 Associated Real-World Activity – Get Worklist

With "Get Worklist" in the patient based Worklist Query dialog, the entered attributes are used to form a worklist request identifier. The response data is used to fill the Patient Registration dialog. The response data are additionally placed in the scheduler database.

### 13.1.2.1.5 Proposed Presentation Contexts – Get Worklist

This RWA will propose the same Presentation Contexts as with "Update Worklist". Please see table in section 13.1.2.1.2.

### 13.1.2.1.6 SOP Specific Conformance – Get Worklist

#### 13.1.2.1.6.1 Search Key Attributes of the Worklist C-FIND

The Artis zee VC13 DICOM worklist SCU supports “narrow worklist queries” with all required search keys. The following tables describe the “narrow query” search keys that the SCU supports.

| Attribute Name | Tag | Matching Key Type | Query Value |
|---|---|---|---|
| Scheduled Procedure Step | | | |
| Scheduled Procedure Step Sequence | (0040,0100) | R | |
| >Scheduled Performing Physician’s Name | (0040,0006) | R | input from UI or <zero length> |
| Requested Procedure | | | |
| Requested Procedure ID | (0040,1001) | O | input from UI or <zero length> |
| Imaging Service Request | | | |
| Accession Number | (0008,0050) | O | input from UI or <zero length> |
| Referring Physician’s Name | (0008,0090) | O | input from UI or <zero length> |
| Visit Status | | | |
| Current Patient Location | (0038,0300) | O | input from UI or <zero length> |
| Patient Identification | | | |
| Patient’s Name | (0010,0010) | R | input from UI or <zero length> |
| Patient ID | (0010,0020) | R | input from UI or <zero length> |

Table 53 Patient based "narrow query" Search Key Attributes

### 13.1.2.1.6.2 Return Key Attributes of the Worklist C-FIND

Please see 13.1.2.1.3 for list of return keys

#### 13.1.2.1.6.3 Status Codes of the Worklist C-FIND

The worklist SCU interprets following status codes:

| Service Status | Meaning | Error Codes | Related Fields |
|---|---|---|---|
| Refused | Out of Resources | A700 | (0000,0902) |
| Failed | Identifier does not match SOP Class | A900 | (0000,0901)<br>(0000,0902) |
| | Unable to process | Cxxx | (0000,0901)<br>(0000,0902) |
| Cancel | Matching terminated due to Cancel request | FE00 | None |
| Success | Matching is complete - No final Identifier is supplied | 0000 | None |
| Pending | Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys | FF00 | Identifier |
| | Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this identifier | FF01 | Identifier |

Table 54 C-FIND-RSP Status

# 14 Implementation Model MPPS

The Modality Performed Procedure Step Service class defines an application-level class of service that facilitates the transfer of procedure, billing and radiation dose information from the imaging modality to the information system. The Performed Procedure Step is created and set by the AE and supplies the SCP with the information about a real-world procedure which is performed on the modality. The Artis zee VC13 DICOM Modality Performed Procedure Step application supports the MPPS service as SCU.

## 14.1 Application Data Flow Diagram

The Artis zee VC13 DICOM network implementation acts as SCU for the Modality Performed Procedure Step SOP Class. The product target Operating System is Windows XP.

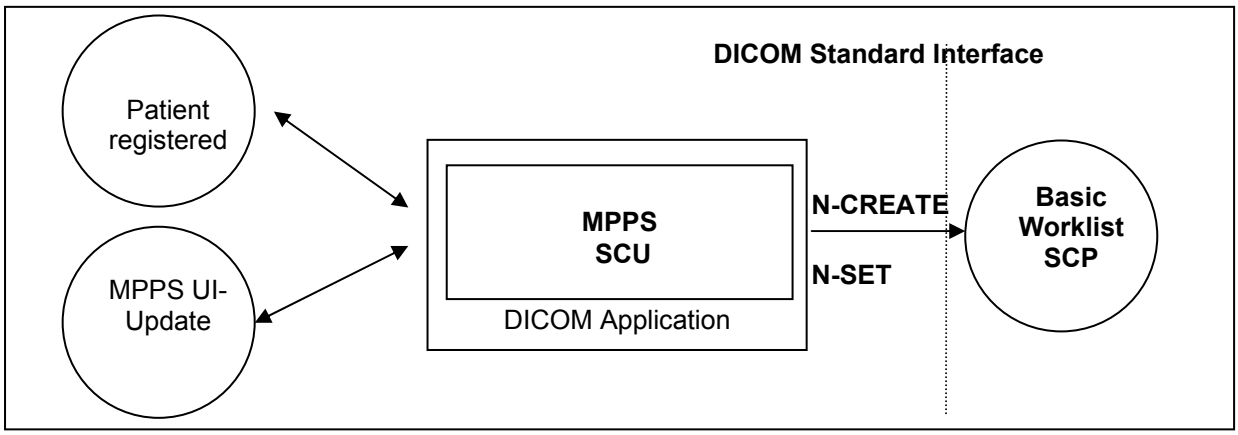


**Figure 8 Artis zee VC13 Application Flow Diagram – MPPS SCU**

## 14.2 Functional Definitions of Application Entities

With registering a Patient (i.e. a Scheduled Procedure Step from Worklist), the Artis zee VC13 DICOM application will create a MPPS Instance and communicate it to the MPPS SCP.

It is configurable to set the states of all related MPPS to "Completed" when a patient is closed. Furthermore, a manual update can be performed with the Artis zee VC13 MPPS user interface. From the user interface it is possible to set the state of the MPPS to “Completed” or “Discontinued”. After that the DICOM application will no longer allow updates on the related MPPS Instance.

The Artis zee VC13 will not only allow a "1:1 -relationship" of Scheduled Procedure Steps and Performed Procedure Steps, but also supports the "simple group-case" (grouping several SPS of the same Requested Procedure) , "complex group-case" (grouping several SPS from different Requested Procedures) and "append case" from the respective IHE-scenarios.

The Artis zee VC13 will support creation of “unscheduled cases” by allowing MPPS Instances to be communicated for locally registered Patients.

## 14.3 Sequencing of real World Activities

An MPPS Update is only possible, if the MPPS Instance was created with Patient Registration before.

# 15 AE Specification MPPS

## 15.1 Modality Performed Procedure Step AE Specification

The Modality Performed Procedure Step SCU (Patient Registration and MPPS UI) provide information about a performed real-world Procedure to a remote SCP (Information System).

SIEMENS Artis zee VC13 DICOM products provide Standard Conformance to the following DICOM V3.0 SOP Class as an SCU:

| SOP Class Name | SOP Class UID |
|---|---|
| Modality Performed Procedure Step | 1.2.840.10008.3.1.2.3.3 |

Table 55 SOP Classes as an SCU

### 15.1.1 Association Establishment Policies

#### 15.1.1.1 General

The creation of MPPS Instance is done automatically by Artis zee VC13 whenever a patient is registered for image acquisition through the Patient Registration dialog.

Further updates on the MPPS data can be done interactively from the related MPPS user interface. The MPPS “Complete” or “Discontinued” states can be set from user interface.

The default PDU size used will be 256 KB.

#### 15.1.1.2 Number of Associations

The Artis zee VC13 DICOM application initiates one association at a time to create or set MPPS instance.

#### 15.1.1.3 Asynchronous Nature

The Artis zee VC13 DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

#### 15.1.1.4 Implementation Identifying Information

| | |
|---|---|
| Implementation Class UID | 1.3.12.2.1107.5.9.20000101 |
| Implementation Version Name | SIEMENS_SWFSYNGO |

Table 56 Implementation Identifying Information

### 15.1.2 Association Initiation Policy

The Artis zee VC13 DICOM Application Entity acts as a Service Class User (SCU) for the

- Modality Performed Procedure Step Service Class (to notify a RIS about status of a procedure while it is performed).

To do so, the Artis zee VC13 will issue a

- N-CREATE DIMSE according to the CREATE Modality Performed Procedure Step SOP Instance operation or a
- N-SET DIMSE to update the contents and state of the MPPS according to the SET Modality Performed Procedure Step Information operation.

### 15.1.2.1 Real World Activity

#### 15.1.2.1.1 Associated Real-World Activity - Patient registered

A patient is registered by the Patient Registration “Exam” action. From this event the trigger to create a MPPS Instance is derived. The related Instance is then immediately communicated to the configured RIS system. An association is established and the MPPS Instance is sent.

#### 15.1.2.1.2 Proposed Presentation Contexts - Patient registered

The Artis zee VC13 DICOM application will propose Presentation Contexts as shown in the following table:

| Presentation Context Table | | | | | |
|---|---|---|---|---|---|
| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg. |
| Name | UID | Name List | UID List | | |
| Modality Performed Procedure Step | 1.2.840.10008.3.1.2.3.3 | Implicit VR Little Endian<br>Explicit VR Little Endian<br>Explicit VR Big Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCU | None |

Table 57 Proposed Presentation Contexts - MPPS

#### 15.1.2.1.3 SOP Specific Conformance Statement- Patient registered

##### 15.1.2.1.3.1 Attributes used for the Performed Procedure Step N-CREATE

The Siemens Artis zee VC13 DICOM Modality Performed Procedure Step SCU informs the remote SCP when the examination of a scheduled procedure step will be performed (i.e. the patient is registered). The N-CREATE message is sent when the examination is started with successful registration of the patient data. The following table describes the supported attributes of a N-CREATE message.

| Attribute Name | Tag | Type | Value |
|---|---|---|---|
| SOP Common | | | |
| Specific Character Set | (0008,0005) | 1C | from MWL or created |
| Performed Procedure Step Relationship | | | |
| Scheduled Step Attribute Sequence | (0040,0270) | 1 | |
| >Study Instance UID | (0020,000D) | 1 | from MWL or created |
| >Referenced Study Sequence | (0008,1110) | 2 | from MWL or <zero length> |
| >>Referenced SOP Class UID | (0008,1150) | 1C | |
| >>Referenced SOP Instance UID | (0008,1155) | 1C | |
| >Accession Number | (0008,0050) | 2 | from MWL or user input |
| >Placer Order Number/Imaging Service Request | (0040,2016) | 3 | from MWL or <zero length> |
| >Filler Order Number/Imaging Service Request | (0040,2017) | 3 | from MWL or <zero length> |
| >Requested Procedure ID | (0040,0001) | 2 | from MWL or user input |
| >Requested Procedure Description | (0032,1060) | 2 | from MWL or <zero length> |

| Attribute Name | Tag | Type | Value |
|---|---|---|---|
| >Scheduled Procedure Step ID | (0040,0009) | 2 | from MWL or <zero length> |
| >Scheduled Procedure Step Description | (0040,0007) | 2 | from MWL or <zero length> |
| >Scheduled Protocol Code Sequence | (0040,0008) | 2 | from MWL or <zero length> |
| >>Code Value | (0008,0100) | 1C | |
| >>Coding Scheme Designator | (0008,0102) | 1C | |
| >>Coding Scheme Version | (0008,0103) | 3 | |
| >>Code Meaning | (0008,0104) | 3 | |
| Patient's Name | (0010,0010) | 2 | from MWL or user input |
| Patient ID | (0010,0020) | 2 | from MWL or user input |
| Patient's Birth Date | (0010,0030) | 2 | from MWL or user input |
| Patient's Sex | (0010,0040) | 2 | from MWL or user input |
| Referenced Patient Sequence | (0008,1120) | 2 | from MWL or <zero length> |
| >Referenced SOP Class UID | (0008,1150) | 1C | |
| >Referenced SOP Instance UID | (0008,1155) | 1C | |
| Performed Procedure Step Information | | | |
| Performed Procedure Step ID | (0040,0253) | 1 | From SPS ID or created |
| Performed Station AE Title | (0040,0241) | 1 | own AE Title |
| Performed Station Name | (0040,0242) | 2 | own hostname |
| Performed Location | (0040,0243) | 2 | from SPS location or <zero length> |
| Performed Procedure Step Start Date | (0040,0244) | 1 | created |
| Performed Procedure Step Start Time | (0040,0245) | 1 | created |
| Performed Procedure Step Status | (0040,0252) | 1 | "IN PROGRESS" |
| Performed Procedure Step Description | (0040,0254) | 2 | from SPS Description or <zero length> |
| Performed Procedure Type Description | (0040,0255) | 2 | <zero length> |
| Procedure Code Sequence | (0008,1032) | 2 | from Requested Procedure Code or <zero length> |
| >Code Value | (0008,0100) | 1C | |
| >Coding Scheme Designator | (0008,0102) | 1C | |
| >Coding Scheme Version | (0008,0103) | 3 | |
| >Code Meaning | (0008,0104) | 3 | |
| Performed Procedure Step End Date | (0040,0250) | 2 | <zero length> |
| Performed Procedure Step End Time | (0040,0251) | 2 | <zero length> |
| Comments on the Performed Procedure Steps | (0040,0280) | 3 | <zero length> |
| Image Acquisition Results | | | |
| Modality | (0008,0060) | 1 | XA |
| Study ID | (0020,0010) | 2 | from Requested Procedure ID or created |
| Performed Protocol Code Sequence | (0040,0260) | 2 | from Scheduled Protocol Code Sequence or <zero length> |
| >Code Value | (0008,0100) | 1C | |
| >Coding Scheme Designator | (0008,0102) | 1C | |
| >Coding Scheme Version | (0008,0103) | 3 | |
| >Code Meaning | (0008,0104) | 3 | |
| Performed Series Sequence | (0040,0340) | 2 | |
| >Performing Physician's Name | (0008,1050) | 2C | from MWL or user input |
| >Operator's Name | (0008,1070) | 2C | User input |
| >Series Instance UID | (0020,000E) | 1C | created |
| >Series Description | (0008,103E) | 2C | <zero length> |
| >Retrieve AE Title | (0008,0054) | 2C | <zero length> |
| >Protocol Name | (0018,1030) | 1C | from organ program |
| >Referenced Image Sequence | (0008,1140) | 2C | <zero length> |
| >Referenced Non-Image Composite SOP Instance Sequence | (0040,0220) | 2C | <zero length> |

| Attribute Name | Tag | Type | Value |
|---|---|---|---|
| **Radiation Dose** | | | |
| Anatomic Structure, Space or Region Sequence | (0008,2229) | 3 | <zero length> |
| Total Time of Fluoroscopy | (0040,0300) | 3 | <zero length> |
| Total Number of Exposures | (0040,0301) | 3 | <zero length> |
| Distance Source to Detector | (0018,1110) | 3 | <zero length> |
| Distance Source to Entrance | (0040,0306) | 3 | <zero length> |
| Entrance Dose | (0040,0302) | 3 | <zero length> |
| Entrance Dose in mGy | (0040,8302) | 3 | <zero length> |
| Exposed Area | (0040,0303) | 3 | <zero length> |
| Image and Fluoroscopy Area Dose Product | (0018,115E) | 3 | <zero length> |
| Comments on Radiation Dose | (0040,0310) | 3 | <zero length> |
| Exposure Dose Sequence | (0040,030E) | 3 | <zero length> |
| **Billing and Material Management Code** | | | |
| Billing Procedure Step Sequence | (0040,0320) | 3 | <zero length> |
| Film Consumption Sequence | (0040,0321) | 3 | |
| >Number of Films | (2100,0170) | 3 | <zero length> |
| >Medium Type | (2000,0030) | 3 | <zero length> |
| >Film Size ID | (2010,0050) | 3 | <zero length> |
| Billing Supplies and Devices Sequence | (0040,0324) | 3 | |
| >Billing Item Sequence | (0040,0296) | 3 | <zero length> |
| >Quantity Sequence | (0040,0293) | 3 | |
| >>Quantity | (0040,0294) | 3 | <zero length> |
| >>Measuring Units Sequence | (0040,0295) | 3 | <zero length> |

Table 58 Performed Procedure Step N-CREATE Attributes

#### 15.1.2.1.3.2 Status Codes of the Performed Procedure Step N-CREATE

The Performed Procedure Step SCU interprets following status codes:

| Service Status | Meaning | Error Codes (0000.0900) |
|---|---|---|
| Failure | Processing Failure | 0110 |
| | No such attribute | 0105 |
| | Invalid attribute value | 0106 |
| | Duplicate SOP Instance | 0111 |
| | No such SOP Instance | 0112 |
| | No such SOP Class | 0118 |
| | Class Instance conflict | 0119 |
| | Missing attribute | 0120 |
| | Missing attribute value | 0121 |
| | Resource limitation | 0213 |
| Success | MPPS Instance created | 0000 |

Table 59 MPPS N-CREATE Response Status

### 15.1.2.1.4 Associated Real-World Activity – MPPS UI-Update

With the MPPS UI the status of the MPPS Instance can be set to “COMPLETED” or “DISCONTINUED”. During performance of the procedure the status will remain “IN PROGRESS”.

### 15.1.2.1.5 Proposed Presentation Contexts – MPPS UI-Update

This RWA will propose the same Presentation Contexts as with “Patient registered”. Please see table in section 15.1.2.1.2.

### 15.1.2.1.6 SOP Specific Conformance Statement – MPPS UI-Update

#### 15.1.2.1.6.1 Attributes used for the Performed Procedure Step N-SET

The Siemens Artis zee VC13 DICOM Modality Performed Procedure Step SCU informs the remote SCP about the performed examination and its status. The N-SET message is sent after each acquisition (status "IN PROGRESS") and per finished examination (finished status “COMPLETED” or incomplete status “DISCONTINUED”). The following table describes the supported attributes of a N-SET message.

| Attribute Name | Tag | Type | Value |
|---|---|---|---|
| Performed Procedure Step Information | | | |
| Performed Procedure Step Status | (0040,0252) | 3 | "IN PROGRESS" during procedure, “COMPLETED” or “DISCONTINUED” for final N-SET |
| Performed Procedure Step Description | (0040,0254) | 3 | from SPS Description or user input |
| Performed Procedure Type Description | (0040,0255) | 3 | User input |
| Procedure Code Sequence | (0008,1032) | 3 | from Requested Procedure |
| >Code Value | (0008,0100) | 1C | |
| >Coding Scheme Designator | (0008,0102) | 1C | |
| >Coding Scheme Version | (0008,0103) | 3 | |
| >Code Meaning | (0008,0104) | 3 | |
| Performed Procedure Step End Date | (0040,0250) | 1 | created |
| Performed Procedure Step End Time | (0040,0251) | 1 | created |
| Image Acquisition Results | | | |
| Performed Protocol Code Sequence | (0040,0260) | 3 | from Scheduled Protocol Code Sequence |
| >Code Value | (0008,0100) | 1C | |
| >Coding Scheme Designator | (0008,0102) | 1C | |
| >Coding Scheme Version | (0008,0103) | 3 | |
| >Code Meaning | (0008,0104) | 3 | |
| Performed Series Sequence | (0040,0340) | 1 | |
| >Performing Physician’s Name | (0008,1050) | 2C | from MWL or user input |
| >Protocol Name | (0018,1030) | 1C | from related SOP Instance |
| >Operator’s Name | (0008,1070) | 2C | user input |
| >Series Instance UID | (0020,000E) | 1C | from related SOP Instance |
| >Series Description | (0008,103E) | 2C | from related SOP Instance |
| >Retrieve AE Title | (0008,0054) | 2C | |
| >Referenced Image Sequence | (0008,1140) | 2C | Series related SOP Instances as items |
| >>Referenced SOP Class UID | (0008,1150) | 1C | |
| >>Referenced SOP Instance UID | (0008,1155) | 1C | |
| >Referenced Standalone SOP Instance Sequence | (0040,0220) | 2C | <zero length> |
| **Radiation Dose** | | | |
| Total Time of Fluoroscopy | (0040,0300) | 3 | |
| Total Number of Exposures | (0040,0301) | 3 | |
| Entrance Dose in mGy | (0040,8302) | 3 | accumulated over complete procedure step |
| Image and Fluoroscopy Area Dose Product | (0018,115E) | 3 | accumulated over complete procedure step (dGy*cm$^2$) |
| Exposure Dose Sequence | (0040,030E) | 3 | on item for each irradiation event (acquistion or fluoro) |
| >Radiation Mode | (0018,115A) | 3 | "PULSED" |
| >KVP | (0018,0060) | 3 | peak KV used for this event (KV) |
| >X-ray Tube Current in µA | (0018,8151) | 3 | tube current used for this event |
| >Exposure Time | (0018,115A) | 3 | time of x-ray in ms for this event |
| **Billing and Material Management Code** | | | |

| Attribute Name | Tag | Type | Value |
|---|---|---|---|
| Film Consumption Sequence | (0040,0321) | 3 | |
| >Number of Films | (2100,0170) | 3 | |
| >Medium Type | (2000,0030) | 3 | |
| >Film Size ID | (2010,0050) | 3 | |

Table 60 Performed Procedure Step N-SET Attributes

#### 15.1.2.1.6.2 Status Codes of the Performed Procedure Step N-SET

The Performed Procedure Step SCU interprets following status codes:

| Service Status | Meaning | Error Codes (0000.0900) |
|---|---|---|
| Failure | Processing Failure: Performed Procedure Step Object may no longer be updated. | 0110 |
| | No such attribute | 0105 |
| | Invalid attribute value | 0106 |
| | No such SOP Instance | 0112 |
| | Invalid Object instance | 0117 |
| | No such SOP Class | 0118 |
| | Class Instance conflict | 0119 |
| | Missing attribute value | 0121 |
| | Resource limitation | 0213 |
| Success | MPPS Instance set | 0000 |

Table 61 MPPS N-SET Response Status

#### 15.1.2.1.6.3 Performed Procedure Step ID without MPPS

Handling of Performed Procedure Step ID in case

- MPPS is not configured or
- Unscheduled case

The attribute “Performed Procedure Step ID” (0040,0235) will be encoded based on "YYYYMMDDHHMMSS". This date and time is based on the time when the first image is acquired. The "Performed Procedure Step ID" stays the same for all acquired or derived images as long as the patient is re-registered. A re-registered patient with a new study or new series within the existing study will get a newly assigned "Performed Procedure Step ID".

# 16 Communication Profiles

## 16.1 Supported Communication Stacks

The Siemens Artis zee VC13 DICOM application provides DICOM TCP/IP Network Communication Support as defined in Part 8 of the DICOM Standard.
The product target Operating System is Windows XP.

### 16.1.1 TCP/IP Stack

The Artis zee VC13 DICOM application uses the TCP/IP stack from the target operating system upon which it executes. It uses the MergeCOM-3 subroutine library from Merge Technologies Inc. that is based on a Berkeley socket interface.

#### 16.1.1.1 API

The Artis zee VC13 DICOM application uses the MergeCOM library that is based on a TCP/IP socket interface.

#### 16.1.1.2 Physical Media Support

The Artis zee VC13 DICOM application is indifferent to the physical medium over which TCP/IP executes; it inherits this from the target operating system upon which it executes.

# 17 Extensions / Specializations / Privatizations

### 17.1.1 Standard Extended / Specialized / Private SOPs

Please refer to Annex A for further information on these topics. A detailed overview is given there.

### 17.1.2 Private Transfer Syntaxes

Not applicable

# 18 Configuration

## 18.1 AE Title/Presentation Address Mapping

To ensure unique identification within the network the hostname should be used as part of the AE Titles (see examples below, hostname = NAME1). The string can be up to 16 characters long and must not contain any extended characters, only 7-bit ASCII characters (excluding Control Characters) are allowed according to DICOM Standard.

**Note**: the current implementation of syngo does not support the full DICOM Standard. Spaces and special characters (like &<> ") in the AE title string are not supported.

### 18.1.1 DICOM Verification

The Verification Service uses the AE configuration of the DICOM Service that is checked with the C-ECHO message. e.g. Verification will use the Storage AE, if initiated to check the configuration of a remote DICOM node.

### 18.1.2 DICOM AE Titles

Within syngo there are local application entity titles for HIS/RIS, Study Transfer and Print. They can be configured via Service-UI in "Configuration / DICOM / General".

#### 18.1.2.1 DICOM Storage AE Title

The DICOM Storage application provides the application entity title which can be configured via Service UI in "Configuration/DICOM/General":

e.g. STU_NAME1

The port number is set to the fixed value of

104

#### 18.1.2.2 DICOM Query/Retrieve AE Title

The DICOM Query/Retrieve application uses the same application entity title as the DICOM Storage AE.

#### 18.1.2.3 DICOM Print AE Title

The DICOM Print application provides the application entity title which can be configured via Service UI in "Configuration/DICOM/General":

e.g. PRI_NAME1

#### 18.1.2.4 DICOM Modality Worklist AE Title

The DICOM Modality Worklist application provides the application entity title which can be configured via Service UI in "Configuration/DICOM/General", e.g. HRI_NAME1.

## 18.2 Configurable Parameters

The Application Entity Titles, host names and port numbers for remote AE are configured using the Artis zee VC13 Service/Installation Tool. For each AET the list of services supported can be configured.

### 18.2.1 Storage, Storage Commitment and Query/Retrieve

The Artis zee VC13 Service/Installation Tool can be used to set the AETs, port-numbers, host-names, IP-addresses and capabilities for the remote nodes (SCPs). The service user can select transfer syntaxes, compression modes and query models for each SCP separately.

The sending of the private SOP Class (Exam Protocol) can be disabled.

For sending or exporting, it can be configured for each destination if resizing (1024, 12 bit; 512, 8 bit) and/or ready-processing (see further information below) shall be used. Resizing and ready-processing can be configured depending on image type.

**Additional configurable parameters for Storage Commitment are:**

- flag to indicate whether the association will be kept open to receive the response or to close the association and be prepared to receive the response on another association.
- time-out which defines how long the association of N-ACTION is kept to receive a N-EVENT-REPORT on the same association. The same value is used to wait for a N-EVENT-REPORT on an other association (default 1 h).

**Additional configurable parameters for ready-processed are:**

- three different packages are defined
  - Package 1: Modality LUT, DSA (subtracting) and pixel shift, edge enhance
  - Package 2: Windowing and invert
  - Package 3: Shutter, Zoom, Roam, Flip, Overlay Graphics/Text (additionally add shutter attributes to header)
- two different modules can be configured for customized ready-processing for each node (N means "ready-process disabled", Y means "ready-process enabled")
- SUB means subtracted display, AB means anatomical background

| Ready Processed | Gray Scale | | | | Transformation | |
|---|---|---|---|---|---|---|
| | MOD LUT | SUB incl. AB incl. Pixel shift | EE | Window incl. Invert | Shutter | Zoom incl. Roam |
| disabled | N | | | N | N | |
| Module 3 | Y | | | N | Y | |
| Module 4 | Y | | | Y | Y | |

Table 62 Ready-processed configuration

### 18.2.2 Print

The Artis zee VC13 Service/Installation Tool can be used to configure the SCP (DICOM-Printer).

These parameters are mandatory to set:

- AET,
- host-name,

- IP-address and
- Port-number.

These parameters have defaults as per configuration file and can be changed:

- default camera (yes/no),
- pixel size,
- additional or changed film sheet formats (e.g. inch 14x14, inch 14x17, ...),
- list with mapping pixel size to each film sheet format,
- minimal density,
- stored printed film jobs,
- media type,
- film destination.

### 18.2.3 Modality Worklist

The Service application can be used to set the AET, port number, host name, IP address, capabilities and time-outs for the remote node (SCP)

**Additional configurable parameters for Modality Worklist Query are:**

- Query Waiting time - the time to wait for the C-FIND-RSP after sending the C-FIND-RQ (default 20 sec.)
- Max Query Match Number - the maximum number of entries accepted in one worklist (default is 200)
- Query Interval: the time between two C-FIND-RQ to the Hospital Information system (default is 60 min., minimum is 3 min., maximum is 1440 min. i.e. 24 hours)
- Broad Worklist Query behavior (two values are defined):
  - Set the AE Title search attribute to the own AE Title, and the Modality search attribute to <zero length>.
  - Set the Modality search attribute to the own modality and the AE Title search attribute to <zero length>.

## 18.3 Default Parameters

This installation tool also uses some default parameters:

- max PDU size set to 262144 Bytes (256 KB)
- time-out for accepting/rejecting an association request: 60 s
- time-out for responding to an association open/close request: 60 s
- time-out for accepting a message over network: 60 s
- time-out for waiting for data between TCP/IP-packets: 60 s

The time-outs for waiting for a Service Request/Response message from the remote node are as follows:

- for Storage SCP/SCU: 600 s

- for Storage Commitment SCU:
  time-out for Response to N-ACTION: 600 s
- for Query/Retrieve SCP/SCU: 600 s

for Print Management SCU:

- time-out for Response to N-SET-RQ: 240 s
- time-out for Response to other Requests: 60 s

# 19 Support of Extended Character Sets

The Artis zee VC13 DICOM application supports the ISO 8859 Latin 1 (ISO-IR 100) character set.

Also the Japanese language character sets JIS X 0201 (ISO-IR 13 Japanese katakana and ISO-IR 14 Japanese romaji), JIS X 0208 (ISO-IR 87 Japanese kanji) and JIS X 0212 (ISO-IR 159 Supplementary Japanese kanji) are supported.

When there is a mismatch between the "Specific Character Set" attribute (0008,0005) and the characters encoded in an IOD received by the system, then the following measures are taken to make the characters DICOM conform:

- Try to import with ISO_IR 100. If ISO_IR 100 fails, convert each illegal character to a ’?’.

# 20 Artis zee VC13 Offline Media Application Profile

Contains a Artis zee VC13specific Application Profile since DICOM does not provide a "General Angio/X-Ray Application Profile" for Storage on "Offline Media".

Structure of this Application Profile is defined in Part 11 of the [DICOM] Standard.

It is needed to describe the requirements for Offline Media Storage of the private IOD (Non-Image IOD).

The profile is shared with LEONARDO Workstation and therefore support of MOD Media is included, even if not used with Artis zee VC13 based systems.

## 20.1 Class and Profile Identification

This document defines an Application Profile Class for X-Ray Modular Angiographic / Radiographic modalities or applications.

The identifier for this class shall be PRI-XAMAS. This class is intended to be used for interchange of extended and private Information Objects via CD-R or re-writeable magneto-optical disk (MOD) offline media between dedicated Angiography, Neuro-Radiology, Radiography applications build from a common architecture.

The specific application profiles in this class are shown in Table 1:

| Application Profile | Identifier | Description |
|---|---|---|
| Universal X-Ray Modular Angio/ Radio System on CD-R | PRI-XAMAS-CD | Handles interchange of Composite SOP Instances and privately defined SOP Instances (Dose Reports, Object Graphics, Quantification Results and more). |

Table 63 PRI-XAMAS Universal Angio/Radio Class Profile

Equipment claiming conformance for this X-Ray Modular Angiographic/Radiographic Application Profile Class shall make a clear statement on handling of the private defined SOP Instances.

## 20.2 Clinical Context

This application profile facilitates the interchange of original acquired and derived images and private data related to them. Typical media interchange would be from in-lab acquisition equipment to dedicated angio workstations and archive systems with specific extensions to handle the private data objects (in both directions).

Additionally, images (from MR, CT, US) used to prepare interventional procedures, multi-modality images (e.g. integrated US) and images derived from primary diagnostic images, such as annotations, quantitative analysis images, reference images may be interchanged via this profile.

### 20.2.1 Roles and Service Class Options

This Application Profile uses the Media Storage Service Class defined in PS 3.4 with the Interchange Option.

The Application Entity shall support one or more of the roles of File Set Creator (FSC), File Set Reader (FSR), and File Set Updater (FSU), defined in PS 3.10.

#### 20.2.1.1 File Set Creator

The Application Entity acting as a File-Set Creator generates a File Set under the PRI-XAMAS Application Profiles.

File Set Creators shall be able to generate the Basic Directory SOP Class in the DICOMDIR file with all the subsidiary Directory Records related to the Image SOP Classes and Private SOP Classes stored in the File Set.

In case of the PRI-XAMAS-CD profile, the FSC shall offer the ability to either finalize the disc at the completion of the most recent write session (no additional information can be subsequently added to the disc) or to allow multi-session (additional information may be subsequently added to the disc).

**Note**

A multiple volume (a logical volume that can cross multiple physical media) is not supported by this Application Profile Class. If a set of Files, e.g., a Study, cannot be written entirely on one CD-R, the FSC will create multiple independent DICOM File-Set such that each File-Set can reside on a single CD-R medium controlled by its individual DICOMDIR file. The user of the FSC can opt to use written labels on the discs to reflect that there is more than one disc for this set of files (e.g., a Study).

#### 20.2.1.2 File Set Reader

The role of the File Set Reader shall be used by Application Entities which receive the transferred File Set.

File Set Readers shall be able to read all the defined SOP Instances files defined for the specific Application Profiles to which a conformance claim is made, using all the defined Transfer Syntaxes.

#### 20.2.1.3 File Set Updater

The role of the File Set Updater shall be used by Application Entities, which receive a transferred File Set and update it by the addition of processed information.

File Set Updaters shall be able to read and update the DICOMDIR file. File-Set Updaters do not have to read the image/private information objects. File-Set Updaters shall be able to generate any of the SOP Instances files defined for the specific Application Profiles to which a conformance claim is made, and to read and update the DICOMDIR file.

In case of the PRI-XAMAS-CD profile, the FSU shall offer the ability to either finalize a disc at the completion of the most recent write session (no additional information can be subsequently added to the disc) or to allow multi-session (additional information may be subsequently added to the disc).

**Note (for CD-R)**

If the disc has not been finalized, the File-Set Updater will be able to update information assuming there is enough space on the disc to write a new DICOMDIR file, the information, and the fundamental CD-R control structures. CD-R control structures are the structures that inherent to the CD-R standards; see PS 3.12

## 20.3 PRI-XAMAS Profiles

### 20.3.1 SOP Classes and Transfer Syntaxes

These Application Profiles are based on the Media Storage Service Class with the Interchange Option.

| Information Object Definition | SOP Class UID | Transfer Syntax UID | FSC | FSR | FSU |
|---|---|---|---|---|---|
| Basic Directory | 1.2.840.10008.1.3.10 | **ELE** | M | M | M |
| X-Ray Angiographic Image | 1.2.840.10008.5.1.4.1.1.12.1 | **JPEG LL P14** | M | M | O |
| | | **ELE** | O | M | O |
| | | **EBE** | O | M | O |
| | | **JPEG Lossy** | O | O | O |
| CT image | 1.2.840.10008.5.1.4.1.1.2 | **ELE** | M | M | O |
| | | **JPEG LL P14** | O | M | O |
| | | **EBE** | O | M | O |
| | | **JPEG Lossy** | O | O | O |
| MR Image | 1.2.840.10008.5.1.4.1.1.4 | **ELE** | M | M | O |
| | | **JPEG LL P14** | O | M | O |
| | | **EBE** | O | M | O |
| | | **JPEG Lossy** | O | O | O |
| CSA Non-Image | 1.3.12.2.1107.5.9.1 | **ELE** | O | M | O |

Table 64 PRI-XAMAS SOP Classes and Transfer Syntaxes

| Abbreviation | Transfer Syntax UID | Transfer Syntax |
|---|---|---|
| **ELE** | 1.2.840.10008.1.2.1 | Explicit VR Little Endian Uncompressed |
| **EBE** | 1.2.840.10008.1.2.2 | Explicit VR Big Endian Uncompressed |
| **JPEG LL P14** | 1.2.840.10008.1.2.4.70 | JPEG Lossless Process 14 (selection value 1) |
| **JPEG Lossy** | 1.2.840.10008.1.2.4.50<br>1.2.840.10008.1.2.4.51 | JPEG Lossy (baseline or extended) |
| **RLE** | 1.2.840.10008.1.2.5 | RLE Lossless |

Table 65 Abbreviations for Transfer Syntaxes

FSC, FSR, FSU – denote the requirements for those roles
O – Optional
M - Mandatory

### 20.3.2 Physical Media and Formats

The PRI-XAMAS-CD Profile requires the 120mm CD-R physical media with the ISO/IEC 9660 Media Format, as defined in PS3.12.

The PRI-XAMAS-MOD23 Profile requires the 130mm 2.3 GB R/W MOD physical medium with the PCDOS Media Format, as defined in PS3.12.

The PRI-XAMAS-MOD41 Profile requires the 130mm 4.1 GB R/W MOD physical medium with the PCDOS Media Format, as approved by DICOM Supplement 62.

### 20.3.3 Directory Information in DICOMDIR

Conforming Application Entities shall include in the DICOMDIR File the Basic Directory IOD containing Directory Records at the Patient and subsidiary levels appropriate to the SOP Classes in the File-set. All DICOM files in the File-set incorporating SOP Instances defined for the specific Application profile, shall be referenced by Directory Records.

**Note**

DICOMDIRs with no directory information are not allowed by this Application Profile. Privately defined IODs will be referenced by "PRIVATE" Directory Records.

### 20.3.3.1 Basic Directory IOD Specialization Option

This Application Profile makes use of optional attributes of the Basic Directory IOD to support recognition of Patient's Storage Service request results in spanning multiple volumes (file sets). Therefore, the File Set Descriptor File can be used and is then referenced by optional Basic Directory IOD attributes. If existent, the specified Descriptor File may be used by FSR applications. Any FSU, FSC shall make a clear Statement if the Descriptor File mechanism is used according to the specialization defined in this Application Profile.

The Descriptor Files shall have the following contents:

One single Line without any control-characters and according to the Basic Character-Set having the following defined text:

"MULTIVOLUME: xx of yy"

xx, yy are replaced by the actual Number of the volume (xx) and the Total Number of Volumes in the set (yy).

If used, the Descriptor File shall have the File ID "README" and reside in same directory level as the DICOMDIR. It is referenced by the attribute [0004,1141] File-set Descriptor File ID having the defined content of "README".

### 20.3.3.2 Additional Keys

File-set Creators and Updaters are required to generate the mandatory elements specified in PS 3.3, Annex F of the DICOM Standard. Table "Table 66 PRI-XAMAS Additional DICOMDIR Keys

" specifies the additional associated keys. At each directory record level other additional data elements can be added, but it is not required that File Set Readers be able to use them as keys. Refer to the Basic Directory IOD in PS 3.3.

| Key Attribute | Tag | Directory Record Level | Type | Notes |
|---|---|---|---|---|
| Date of Birth | (0010,0030) | PATIENT | 2C | required, if present in SOP Instance |
| Patient's Sex | (0010,0040) | PATIENT | 2C | required, if present in SOP Instance |
| Series Date | (0008,0021) | SERIES | 3 | |
| Series Time | (0008,0031) | SERIES | 3 | |
| Institute Name | (0008,0080) | SERIES | 2C | required, if present in SOP Instance |
| Institution Address | (0008,0081) | SERIES | 2C | required, if present in SOP Instance |
| Series Description | (0008,103E) | SERIES | 3 | |
| Performing Physician's Name | (0008,1050) | SERIES | 2C | required, if present in SOP Instance |
| Image Type | (0008,0008) | IMAGE | 1C | required, if present in SOP Instance |
| SOP Class UID | (0008,0016) | IMAGE | 3 | |
| SOP Instance UID | (0008,0018) | IMAGE | 3 | |
| Image Date | (0008,0023) | IMAGE | 3 | |
| Image Time | (0008,0033) | IMAGE | 3 | |
| Referenced Image Sequence | (0008,1140) | IMAGE | 1C | required, if present in SOP Instance |
| > Referenced SOP Class UID | (0008,1150) | | | |
| > Referenced SOP Instance UID | (0008,1155) | | | |
| Image Position (Patient) | (0020,0032) | IMAGE | 2C | required, if present in SOP Instance |

| Key Attribute | Tag | Directory Record Level | Type | Notes |
|---|---|---|---|---|
| Image Orientation (Patient) | (0020,0037) | IMAGE | 2C | required, if present in SOP Instance |
| Frame of Reference UID | (0020,0052) | IMAGE | 2C | required, if present in SOP Instance |
| Rows | (0028,0010) | IMAGE | 3 | |
| Columns | (0028,0011) | IMAGE | 3 | |
| Pixel Spacing | (0028,0030) | IMAGE | 1C | required, if present in SOP Instance |
| Calibration Image | (0050,0004) | IMAGE | 2C | required, if present in SOP Instance |
| Icon Image Sequence | (0088,0200) | IMAGE | 3 | Required for Image SOP Classes |
| > Samples per Pixel | (0028,0002) | | | 1 |
| > Photometric Interpretation | (0028,0004) | | | MONOCHROME2 |
| > Rows | (0028,0010) | | | 128 for XA, 64 for others |
| > Columns | (0028,0011) | | | 128 for XA, 64 for others |
| > Bits Allocated | (0028,0100) | | | 8 |
| > Bits Stored | (0028,0101) | | | 8 |
| > High Bit | (0028,0102) | | | 7 |
| > Pixel Representation | (0028,0103) | | | 0 |
| > Pixel Data | (7FE0,0010) | | | Icon Image |

Table 66 PRI-XAMAS Additional DICOMDIR Keys

#### 20.3.3.3 Private Directory Record Keys

Private Directory Records are supported by this Application Profile Class at the following Level - IMAGE. The PRIVATE Directory Records will have required elements in addition to the mandatory elements specified in PS 3.3.

The following table will list the additional required keys for PRIVATE Directory Records:

| Key Attribute | Tag | Directory Record Level | Type | Notes |
|---|---|---|---|---|
| Private Record UID | (0004,1432) | PRIVATE | 1 | See Conformance Statement |
| SOP Class UID | (0008,0016) | PRIVATE | 1C | required, if present in SOP Instance |
| SOP Instance UID | (0008,0018) | PRIVATE | 1C | required, if present in SOP Instance |
| Image Type | (0008,0008) | PRIVATE | 3 | |
| Acquisition Date | (0008,0022) | PRIVATE | 3 | |
| Acquisition Time | (0008,0032) | PRIVATE | 3 | |
| Acquisition Number | (0020,0012) | PRIVATE | 3 | |
| CSA Data Type | (0029,xx08) | PRIVATE | 1 | private owner code = SIEMENS CSA NON-IMAGE |
| CSA Data Version | (0029,xx09) | PRIVATE | 3 | private owner code = SIEMENS CSA NON-IMAGE |

Table 67 PRI-XAMAS Additional PRIVATE Record Keys

#### 20.3.3.4 Icon Images

Directory Records of type SERIES or IMAGE may include Icon Images. The Icon Image pixel data shall be as specified in PS 3.3 "Icon Image Key Definition", and restricted such, that Bits Allocated (0028,0100) and Bits Stored (0028,0101) shall be equal 8, and Rows (0028,0010) and Columns (0028,0011) shall be equal to 128 for XA Images and 64 for all other Images. The Photometric Interpretation (0028,0004) shall always be restricted to "MONOCHROME2".

PRIVATE Directory Records will not contain Icon Image information.

### 20.3.4 Other Parameters

This section defines other parameters common to all specific Application Profiles in the PRI-XAMAS class which need to be specified in order to ensure interoperable media interchange.

### 20.3.4.1 Multi-Frame JPEG Format

The JPEG encoding of pixel data shall use Interchange Format (with table specification) for all frames.

### 20.3.4.2 Attribute Value Precedence

The values of attributes contained in a Detached Patient Management SOP Instance referenced by a DICOMDIR PATIENT Directory Record shall take precedence over the values of those attributes contained in the SOP Instance referenced by a subsidiary Directory Record. The DICOMDIR Directory Records shall have key attribute values in accordance with this precedence.

**Note**

This allows patient identification and demographic information to be updated without changing the composite Image IOD files. The DICOMDIR file thus is critical in establishing the link between the updated information and the image. As an example, at the time an Image file was written, the patient's name therein was incorrect, or inconsistent with the Hospital Information System records. Subsequently, a Detached Patient Management file with the corrected name is added to the file-set. The FSR should use the name from the Patient File rather than in the Image File.

# 21 Application Profile Conformance Statement

This chapter defines the Conformance Statement to all “Offline Media Application Profiles (incl. private extensions)” supported by the Artis zee VC13 archive options.

Those application profiles supported shall be:

- 1024 Extended Cardiac Application Profile
- General Purpose CDR Profiles
- Artis zee VC13private Application Profile

## 21.1 Introduction

### 21.1.1 Purpose

This DICOM Conformance Statement is written according to part PS 3.2 of [DICOM] .

The applications described in this conformance statement are the SIEMENS Artis zee VC13 based on *syngo*® software[a]. The Artis zee VC13 DICOM offline media storage service implementation acts as FSC, FSU and/or FSR for the specified application profiles and the related SOP Class instances.

### 21.1.2 Scope

This DICOM Conformance Statement refers to SIEMENS Artis zee VC13

### 21.1.3 Definitions, Abbreviations

#### 21.1.3.1 Definitions

| | |
|---|---|
| DICOM | Digital Imaging and Communications in Medicine |
| DIMSE | DICOM Message Service Element |
| DIMSE-C | DICOM Message Service Element with Composite information objects |

### 21.1.4 Abbreviations

| | |
|---|---|
| AE | DICOM Application Entity |
| ASCII | American Standard Code for Information Interchange |
| CD, CD-R | Compact Disk Recordable |
| DB | Database |
| FSC | File Set Creator |
| FSR | File Set Reader |
| FSU | File Set Updater |
| IOD | DICOM Information Object Definition |
| ISO | International Standard Organization |
| MAS or M.A.S. | AX-Workstation (for Angiographic/Radiographic viewing) |
| NEMA | National Electrical Manufacturers Association |
| O | Optional Key Attribute |
| PDU | DICOM Protocol Data Unit |
| R | Required Key Attribute |
| RWA | Real-World Activity |
| U | Unique Key Attribute |

[a] *syngo* is a registered trademark of Siemens AG.

### 21.1.5 References

[DICOM] Digital Imaging and Communications in Medicine (DICOM), NEMA PS 3.1-18

### 21.1.6 Remarks

DICOM and this Conformance Statement, by itself, does not guarantee interoperability. However, the Conformance Statement facilitates a first-level validation for interoperability between different applications supporting the same DICOM functionality as SCU and SCP, respectively.

This Conformance Statement is not intended to replace validation with other DICOM equipment to ensure proper exchange of information intended.

The scope of this Conformance Statement is to facilitate communication with Siemens and other vendors' Medical equipment. The Conformance Statement should be read and understood in conjunction with the DICOM Standard [DICOM] . However, by itself it is not guaranteed to ensure the desired interoperability and a successful interconnectivity.

The user should be aware of the following important issues:

- Interoperability
  Interoperability refers to the ability of application functions, distributed over two or more systems, to work successfully together. The integration of medical devices into a networked environment may require application functions that are not specified within the scope of DICOM. Consequently, using only the information provided by this Conformance Statement does not guarantee interoperability of SIEMENS equipment with non-SIEMENS equipment. It is the user's responsibility to analyze thoroughly the application requirements and to specify a solution that integrates SIEMENS equipment with non-SIEMENS equipment.
- Validation
  SIEMENS equipment has been carefully tested to assure that the actual implementation of the DICOM interface corresponds with this Conformance Statement. Where SIEMENS equipment is linked to non-SIEMENS equipment, the first step is to compare the relevant Conformance Statements. If the Conformance Statements indicate that successful information exchange should be possible, additional validation test will be necessary to ensure the functionality, performance, accuracy and stability of image and image related data. It is the responsibility of the user (or user's agent) to specify the appropriate test suite and to carry out the additional validation tests.
- New versions of the DICOM Standard
  The DICOM Standard will evolve in future to meet the user's growing requirements and to incorporate new features and technologies. SIEMENS is actively involved in this evolution and plans to adapt its equipment to future versions of the DICOM Standard. In order to do so, SIEMENS reserves the right to make changes to its products or to discontinue its delivery. The user should ensure that any non-SIEMENS provider linking to SIEMENS equipment, also adapts to future versions of the DICOM Standard. If not, the incorporation of DICOM enhancements into SIEMENS equipment may lead to loss of connectivity (in case of networking) and incompatibility (in case of media).

## 21.2 Implementation Model

### 21.2.1 Application Data Flow Diagram

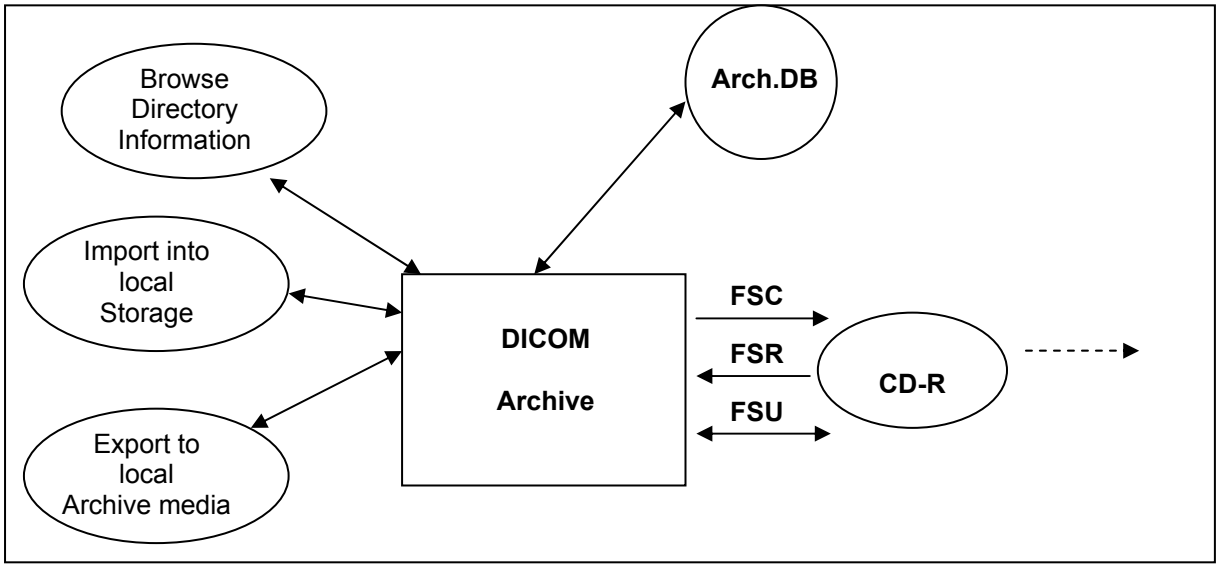


**Figure 9 Application Data Flow Diagram**

The DICOM archive application will serve as an interface to the CD-R offline medium device. It serves interfaces to include the offline media directory into the browser and to copy SOP instances to a medium or retrieve SOP Instances from medium into local storage.

The DICOM Archive application will support the 120mm CD-R medium.

The FSU role will update new SOP Instances only to media with pre-existing File-sets conforming to the Application Profiles supported.

The contents of the DICOMDIR will be temporarily stored in Archive-Database.

### 21.2.2 Functional Definitions of AEs

The Artis zee VC13 DICOM offline media storage application consists of the DICOM Archive application entity serving all interfaces to access offline media. The DICOM Archive application is capable of

1. creating a new File-set onto an unwritten medium (Export to…).
2. updating an existing File-set by writing new SOP Instances onto the medium (Export to...).
3. importing SOP Instances from the medium onto local storage
4. reading the File-sets DICOMDIR information into temporary database and pass it to display applications.

### 21.2.3 Sequencing of Real-World Activities

The DICOM Archive application will not perform updates before the Directory information of the DICOMDIR is completely read.

When performing updates, the SOP instances are checked for existence before updating. Duplicate instances will be avoided.

### 21.2.4 File Meta Information Options

| | |
|---|---|
| Implementation Class UID | 1.3.12.2.1107.5.9.20000101 |
| Implementation Version Name | SIEMENS_SWFSYNGO |

Table 68 File Meta Information Options

## 21.3 AE Specifications

### 21.3.1 DICOM Archive Specification

The DICOM Archive provides Standard conformance to Media Storage Service Class (Interchange Option). In addition Augmented conformance is provided to store extra data attributes important for the full feature support of the Artis zee VC13 product SW. Details are listed in following Table:

| Application Profiles Supported | Real-World Activity | Role | SC Option |
|---|---|---|---|
| PRI-XAMAS-CD<br>AUG-XA1K-CD *1 | Browse Directory Information | FSR | Interchange |
| | Import into local Storage | FSR | Interchange |
| | Export to local Archive Media | FSC, FSU | Interchange |
| STD-GEN-CD<br>STD-XABC-CD<br>STD-XA1K-CD | Browse Directory Information | FSR | Interchange |
| | Import into local Storage | FSR | Interchange |

*1 – With no Private SOP Class used, the PRI-XAMAS-CD profile definitions are appropriate to describe the augmentation of the related -STD Profiles.

Table 69 Application profiles, Activities, and Roles for DICOM Archive

On Artis zee VC13 based Cardiac Systems the Private Extended MAS Profile (PRI-XAMAS-CD) will be preferably used by the system. The General Purpose Interchange Profile (STDGEN-CD), Basic Cardiac Profile (STD-XABC-CD) and 1024 X-Ray Angiographic Profile (STD-XA1K-CD) will be supported with read capability of the related media.

#### 21.3.1.1 File Meta Information for the Application Entity

The Source Application Entity Title is set by configuration. See Chapter “Configuration” for details.

#### 21.3.1.2 Real-World Activities for this Application Entity

##### 21.3.1.2.1 Real-World Activity: Browse Directory Information

The DICOM Archive application acts as FSR using the interchange option when requested to read the media directory.

The DICOM archive application will read the DICOMDIR and insert those directory entries, that are valid for the application profiles supported, into a local database. The database can the then be used for browsing media contents.

**Note**

Icon Image SQ is also supported in DICOMDIR. But only those Icon Images with Bits Allocated (0028,0100) equal to 8 and size of 64x64 or 128x128 pixels are imported into database and are visible in the Browser.

#### 21.3.1.2.1.1 Application Profiles for the RWA: Browse Directory Information

See Table in Chapter 21.3.1 for the Application Profiles listed that invoke this Application Entity for the Browse Directory Information RWA.

### 21.3.1.2.2 Real-World Activity: Import into local Storage

The DICOM Archive application acts as FSR using the interchange option when requested to read SOP Instances from the medium into the local storage.

The SOP Instance selected from the media directory will be copied into the local storage. Only SOP Instances, that are valid for the application profile supported and are listed as supported by the Storage SCP Conformance section (see chapter 5.1.3.1.2), can be retrieved from media storage. This is due to the fact that the Browse Directory Information will filter all SOP Instances not matching the Application profiles supported.

***During operation no "Attribute Value Precedence" is applied to the SOP Instances. Detached Patient Management is not supported.***

For media conforming to the STD-GEN-CD Profile the following SOP classes will be supported as an FSR:

| Information Object Definition | SOP Class UID | Transfer Syntax UID |
|---|---|---|
| X-Ray Angiographic Image | 1.2.840.10008.5.1.4.1.1.12.1 | Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1 |
| CT image | 1.2.840.10008.5.1.4.1.1.2 | Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1 |
| MR Image | 1.2.840.10008.5.1.4.1.1.4 | Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1 |
| CSA Non-Image | 1.3.12.2.1107.5.9.1 | Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1 |

Table 70 STD-GEN-CD Supported SOP Classes for FSR Role

#### 21.3.1.2.2.1 Application Profiles for the RWA: Import into local Storage

See Table in section 21.3.1 for the Application Profiles listed that invoke this Application Entity for the Import into Local Storage RWA.

### 21.3.1.2.3 Real-World Activity: Export to local Archive Media

The DICOM Archive application acts as FSU (for media with existing DICOM file-set) or FSC (media not initialized) using the interchange option when requested to copy SOP Instances from the local storage to local Archive Medium.

The DICOM Archive application will receive a list of SOP Instances to be copied to the local archive medium. According to the state of the medium inserted (new medium, Medium with DICOM file-set) the validity of the SOP Instances according to the applicable profile is checked. Only valid SOP Instances are accepted.

When the DICOM archive application is requested to copy SOP Instances the preferred application profile according configuration (AUG-XA1K-CD or PRI-XAMAS-CD) will be used to validate and copy the referred SOP Instances. When creating a new file-set no Descriptor File will be allocated and the related ID is not used.

The DICOM archive application will not close the medium.

With the "Export" function a copy of images in Cardiac Format (512x512, 8Bit) can be written onto medium (configurable). Please refer to the Storage section (5.1.2.1.6) RWA description to learn more about the type of conversion that is performed on the Instances.

#### 21.3.1.2.3.1 Application Profiles for the RWA: Export to local Archive Media

See Table in section 21.3.1 for the Application Profiles listed that invoke this Application Entity for the Export to local Archive Media RWA.

## 21.4 Augmented and Private Profiles

### 21.4.1 Augmented Application Profiles

With no private Siemens Non-Images stored onto Medium, the definitions of the PRI-XAMAS-CD Profile are applicable to denote the augmentations for the STD-XA1K-CD Standard Profile.

Storage of Private Information Objects will only be supported with reference to a Private Application Profile (see next section).

### 21.4.2 Private Application Profiles

#### 21.4.2.1 PRI-XAMAS-CD

The DICOM Archive application is conforming to the PRI-XAMAS-CD application profile (see chapter 20.3). Please refer to next section for detailed definition of SOP classes supported in accordance to this Application Profile.

## 21.5 Extensions, Specialization and Privatization of SOP Classes and Transfer Syntaxes

The SOP Classes listed refer to those created by the equipment to which this conformance Statement is related to.

### 21.5.1 SOP Specific Conformance Statement for Basic Directory

The Basic Directory Header will not contain Information to indicate the current medium is part of a sequence of multiple media holding the Objects of one patient/study in total.

#### 21.5.1.1 Extension, Specialization for SIEMENS Non-Image Objects

According to the PRI-XAMAS Application Profile Class the usage of the Private Creator UIDs and further optional keys for the Directory Records referring to SIEMENS Non-Image Objects are listed in the following tables.

| Attribute | Tag | Value used |
|---|---|---|
| Private Record UID | (0004,1432) | 1.3.12.2.1107.5.9.1 |
| SOP Class UID | (0008,0016) | 1.3.12.2.1107.5.9.1 |

Table 71 Extension, Specialization for SIEMENS Non-Image Objects

For those “Non-Images” no Icon Image Sequence will be generated.

## 21.6 Configuration

### 21.6.1 AE Title Mapping

#### 21.6.1.1 DICOM Media Storage AE Title

The DICOM Storage application provides the application entity title:

CsaImageManager

## 21.7 Support of Extended Character Sets

The Siemens Artis zee VC13 DICOM archive application supports the ISO 8859 Latin 1 (ISO-IR 100) character set.

Also the Japanese language character sets JIS X 0201 (ISO-IR 13 Japanese katakana and ISO-IR 14 Japanese romaji), JIS X 0208 (ISO-IR 87 Japanese kanji) and JIS X 0212 (IOS-IR 159 Supplementary Japanese kanji) are supported.

When there is a mismatch between the SCS tags (0008,0005) and the characters in an IOD received by the system, then the following measures are taken to make the characters DICOM conform:

- Try to import with ISO_IR 100. If ISO_IR 100 fails, convert each illegal character to a '?'.

# Annex A: Additional Information

## A.1 SIEMENS Private Non-Image IOD

For encoding binary data-streams not representing image data, Siemens has created a private "Non-Image IOD" according to the rules governed by the DICOM Standard. The following section will define this Private IOD. It can be communicated with Network Storage Service and Offline Media Storage Services.

The Siemens "Non-Image IOD" is identified by a private Non-Image Storage SOP Class UID.

| Private Non-Image Object | Private Non-Image IOD |
|---|---|
| CSA Non-Image | 1.3.12.2.1107.5.9.1 |

Table 72 SIEMENS Private Non-Image IOD

### A.1.1 Siemens Non-Image IOD – E-R Model

The E-R model in A.1.2 depicts those components of the DICOM Information Model which directly refer to the Siemens Non-Image IOD. The Frame of Reference IE, Overlay IE, Modality Lookup-Table IE, VOI Lookup-Table IE and Curve IE are not components of the Siemens Non-Image IOD.

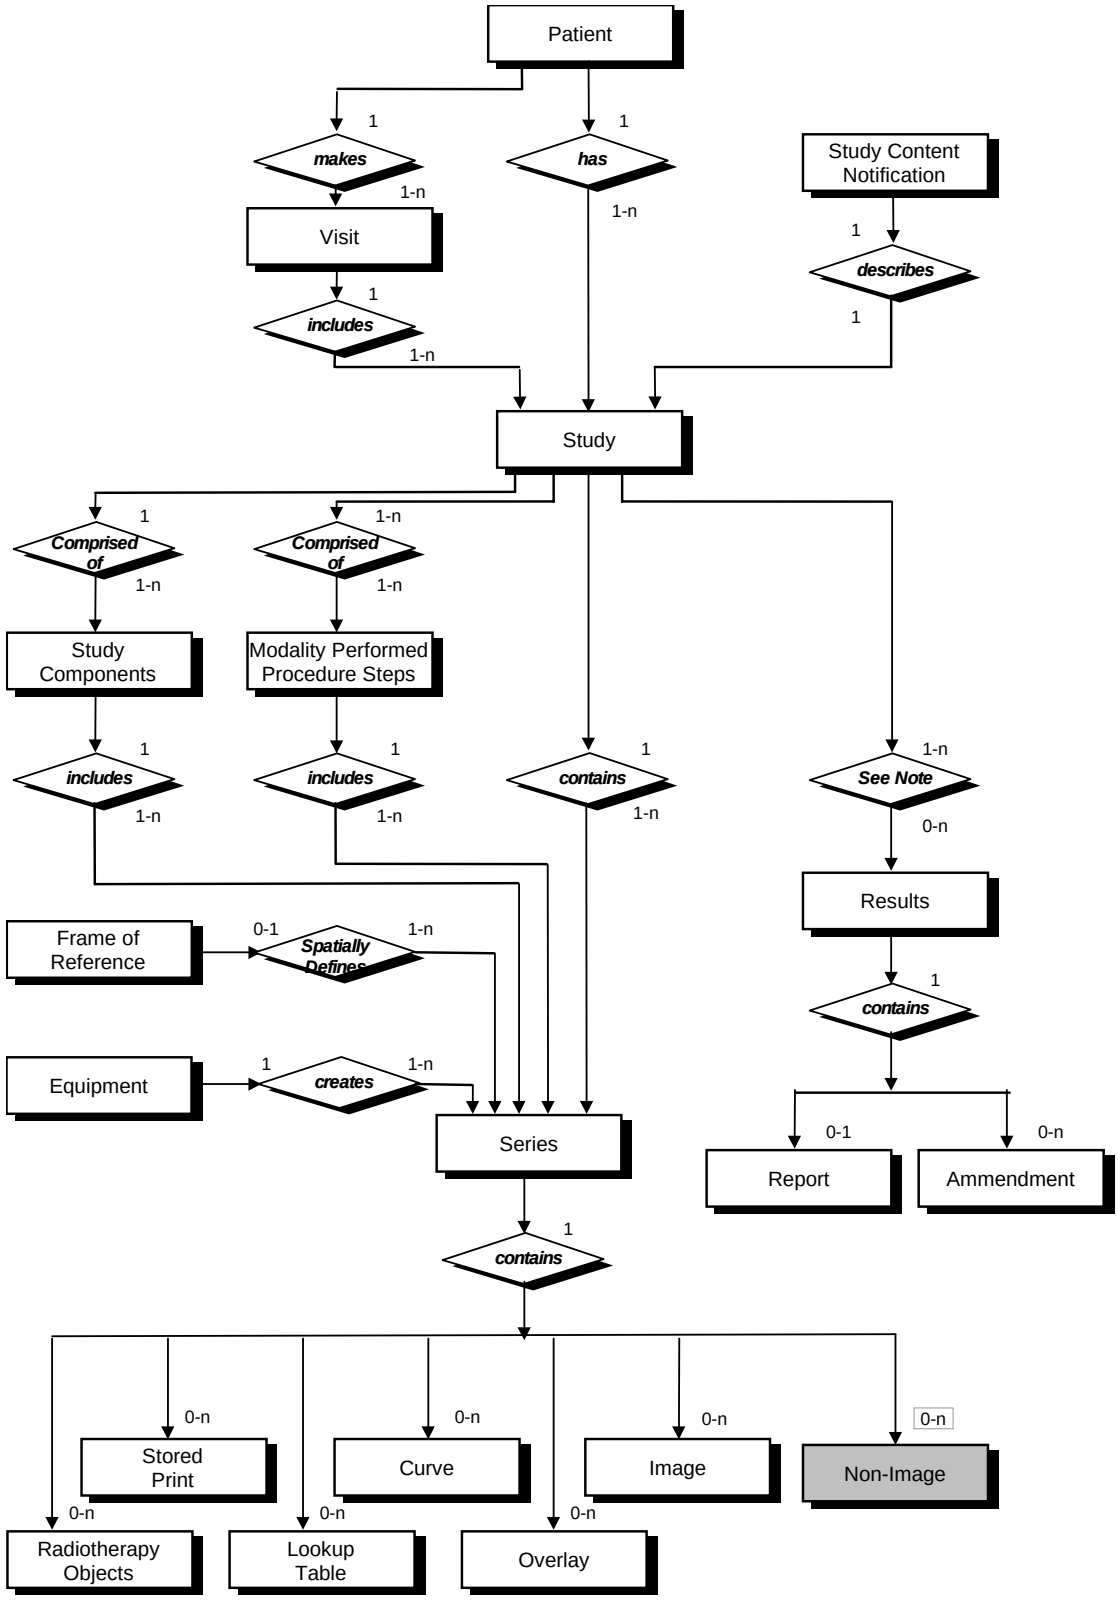


**Figure 10 DICOM Information Model**

### A.1.2 Siemens Non-Image IOD - Module Table

| IE | Module | Reference | Usage |
|---|---|---|---|
| Patient | Patient | [1] PS3.3 C.7.1.1 | M |
| Study | General Study | [1] PS3.3 C.7.2.1 | M |
| | Patient Study | [1] PS3.3 C.7.2.2 | U |
| Series | General Series | [1] PS3.3 C.7.3.1 | M |
| Equipment | General Equipment | [1] PS3.3 C.7.5.1 | U |
| CSA | CSA Image Header | A.2.1 | U |
| | CSA Series Header | A.2.2 | U |
| | MEDCOM Header | A.2.3 | U |
| | CSA Non-Image | A.1.3.1 | M |
| | SOP Common | [1] PS3.3 C.12.1 | M |

Table 73 CSA Non-Image IOD Modules

### A.1.3 Siemens Non-Image IOD - Modules

#### A.1.3.1 CSA Non-Image Attributes

The table in this section contains private IOD Attributes that describe CSA Non-Images.

| Attribute Name | Tag | Owner | Type | Notes |
|---|---|---|---|---|
| Image Type | (0008,0008) | - | 3 | Image identification characteristics. |
| Acquisition Date | (0008,0022) | - | 3 | The date the acquisition of data that resulted in this data set started. |
| Acquisition Time | (0008,0032) | - | 3 | The time the acquisition of data that resulted in this data set started. |
| Conversion Type | (0008,0064) | - | 3 | Describes the kind of image conversion. Defined Terms: DV = Digitized Video, DI = Digital Interface, DF = Digitized Film, WSD = Workstation. |
| Referenced Image Sequence | (0008,1140) | - | 3 | A sequence which provides reference to a set of Image SOP Class/Instance identifying other images significantly related to this data set. Encoded as sequence of items: (0008,1150) and (0008,1155). |
| Derivation Description | (0008,2111) | - | 3 | A text description of how this data set was derived. |
| Source Image Sequence | (0008,2112) | - | 3 | A Sequence which identifies the set of Image SOP Class/Instance pairs of the Images which were used to derive this data set. Zero or more Items may be included in this Sequence. Encoded as sequence of items: (0008,1150) and (0008,1155). |
| Patient Position | (0018,5100) | - | 3 | Patient position descriptor relative to the equipment. |
| Acquisition Number | (0020,0012) | - | 3 | A number identifying the single continuous gathering of data over a period of time which resulted in this data set. |
| Instance Number | (0020,0013) | - | 3 | A number that identifies this data set. |
| Frame of Reference UID | (0020,0052) | - | 3 | Uniquely identifies the frame of reference for a Series. |
| Image Comments | (0020,4000) | - | 3 | User-defined comments about the image. |
| Quality Control Image | (0028,0300) | - | 3 | Indicates whether or not this image is a quality control or phantom image. If this Attribute is absent, then the image may or may not be a quality control or phantom image. Enumerated Values: YES, NO. |

| Attribute Name | Tag | Owner | Type | Notes |
|---|---|---|---|---|
| Burned in Annotation | (0028,0301) | - | 3 | Indicates whether or not image contains sufficient burned in annotation to identify the patient and date the image was acquired.<br>If this Attribute is absent, then the image may or may not contain burned in annotation.<br>Enumerated Values: YES, NO. |
| Lossy Image Compression | (0028,2110) | - | 3 | Specifies whether an Image has undergone lossy compression.<br>Enumerated Values: 00 = Image has not been subjected to lossy compression, 01 = Image has been subjected to lossy compression. |
| Lossy Image Compression Ratio | (0028,2112) | - | 3 | Describes the approximate lossy compression ratio(s) that have been applied to this image.<br>May be multi valued if successive lossy compression steps have been applied. |
| CSA Data Type | (0029,xx08) | SIEMENS CSA NON-IMAGE | 1 | CSA Data identification characteristics.<br>Defined Terms:<br>BSR REPORT = Exam Protocol Data<br>RT3D CONFIG = InSpaceIS Data |
| CSA Data Version | (0029,xx09) | SIEMENS CSA NON-IMAGE | 3 | Version of CSA Data Info (0029,xx10) format and CSA Non-Image Data (7FE1,xx10) format. |
| CSA Data Info | (0029,xx10) | SIEMENS CSA NON-IMAGE | 3 | Information to describe the CSA Data (7FE1,xx10). |
| CSA Data | (7FE1,xx10) | SIEMENS CSA NON-IMAGE | 2 | Binary data as byte stream. |

Table 74 CSA Non-Image Attributes

## A.2 Siemens Standard Extended Modules

| IE | Module | Reference | Usage | Note |
|---|---|---|---|---|
| Image | CSA Image Header | A.2.1 | U | private GG information |
| | CSA Series Header | A.2.2 | U | |
| | MEDCOM Header | A.2.3 | U | private *syngo* information |
| | MEDCOM OOG | A.2.4 | U | if object graphics is attached to image |
| | Edge Enhancement | A.2.5 | U | private Filter Information |
| | Angio Viewing | A.2.6 | U | private Viewing information |
| | Angio Acquisition | A.2.7 | U | additional private Information about image Acquisition |
| | Angio Quantification | A.2.8 | U | if image is a Quant Report |
| | Original Image Info | A.2.9 | U | if derived image |

Table 75 CSA Image IOD Modules

### A.2.1 MEDCOM Header Module

The table in this section contains private IOD Attributes that describe MEDCOM Header:

| Attribute Name | Tag | Owner | Type | Notes |
|---|---|---|---|---|
| MedCom Header Type | (0029,xx08) | SIEMENS MEDCOM HEADER | 1C | MedCom Header identification characteristics.<br>Defined Terms:<br>MEDCOM 1<br>(Required if MedCom Header Info (0029,xx10) present.) |
| MedCom Header Version | (0029,xx09) | SIEMENS MEDCOM HEADER | 2C | Version of MedCom Header Info (0029,xx10) format.<br>(Required if MEDCOM Header Info (0029,xx10) present.) |
| MedCom Header Info | (0029,xx10) | SIEMENS MEDCOM HEADER | 3 | Manufacturer model dependent information.<br>The value of the attribute MedCom Header Info (0029,xx10) can be build up in any user defined format. |
| MedCom History Information | (0029,xx20) | SIEMENS MEDCOM HEADER | 3 | MedCom defined Patient Registration history information. See A.2.3.1. |
| PMTF Information 1 | (0029,xx31) | SIEMENS MEDCOM HEADER | 3 | Transformation Information |
| PMTF Information 2 | (0029,xx32) | SIEMENS MEDCOM HEADER | 3 | Transformation Information |
| PMTF Information 3 | (0029,xx33) | SIEMENS MEDCOM HEADER | 3 | Transformation Information |
| PMTF Information 4 | (0029,xx34) | SIEMENS MEDCOM HEADER | 3 | Transformation Information |
| PMTF Information 5 | (0029,xx35) | SIEMENS MEDCOM HEADER | 3 | Transformation Information |
| Application Header Sequence | (0029,xx40) | SIEMENS MEDCOM HEADER | 3 | Sequence of Application Header items. Zero or more items are possible. |
| >Application Header Type | (0029,xx41) | SIEMENS MEDCOM HEADER | 1C | Application Header identification characteristics.<br>Required, if Sequence is sent. |
| >Application Header ID | (0029,xx42) | SIEMENS MEDCOM HEADER | 3 | Identification of an application header |
| >Application Header Version | (0029,xx43) | SIEMENS MEDCOM HEADER | 3 | Version of CSA Series Header Info (0029,xx44) format. |
| >Application Header Info | (0029,xx44) | SIEMENS MEDCOM HEADER | 3 | Application dependent information. |
| Workflow Control Flags | (0029,xx50) | SIEMENS MEDCOM HEADER | 3 | Eight free definable flags. |
| Archive Management Flag Keep Online | (0029,xx51) | SIEMENS MEDCOM HEADER | 3 | Flag to control remote archive management system to keep the image always online (also when already archived).<br>Enumerated Values:<br>00 = remote control not required<br>01 = keep image online |
| Archive Management Flag Do Not Archive | (0029,xx52) | SIEMENS MEDCOM HEADER | 3 | Flag to control remote archive management system not to archive the related image.<br>Enumerated Values:<br>00 = remote control not required<br>01 = don't archive image |

| Attribute Name | Tag | Owner | Type | Notes |
|---|---|---|---|---|
| Image Location Status | (0029,xx53) | SIEMENS MEDCOM HEADER | 3 | Image location status to control retrieving.<br>Defined Terms:<br>ONLINE = retrieving has to be done as usual,<br>NEARLINE = move request to SCP and delay according to value of Estimated Retrieve Time (0029,xx54),<br>OFFLINE = invoking a retrieve operation initiates an operator request,<br>INVALID = invoking a retrieve operation would always result in an error. |
| **Attribute Name** | **Tag** | **Owner** | **Type** | **Notes** |
| Estimated Retrieve Time | (0029,xx54) | SIEMENS MEDCOM HEADER | 3 | Estimated retrieve time in seconds. A value less then zero (< 0) indicates location is OFFLINE or INVALID. |
| Data Size of Retrieved Images | (0029,xx55) | SIEMENS MEDCOM HEADER | 3 | Data size of images in MByte. |
| Series Workflow Status | (0029,xx60) | SIEMENS MEDCOM HEADER2 | 3 | |

Table 76 MEDCOM Header Modules

### A.2.1.1 MEDCOM History Information

The value of the attribute MEDCOM History Information (0029,xx20) is defined in the following way:

| Part | Name | Type | Bytes | Notes |
|---|---|---|---|---|
| header | Identifier | string | 32 | Always “CSA HISTORY” |
| | Version | string | 32 | e.g. “V1.10” |
| n Items | Class Name | string | 64 | |
| | Modification String | string | 1024 | |

Table 77 MEDCOM History Information

## A.2.2 MEDCOM OOG Module

The table in this section contains private IOD Attributes that describe MEDCOM Object Oriented Graphics (OOG). This module is used whenever object graphics is drawn on the image and need to be stored as graphic object properties. Given the condition that the module contents was not removed by other modalities, the graphic objects remain re-animatable if such an image was transferred and is then retrieved back

| Attribute Name | Tag | Owner | Type | Notes |
|---|---|---|---|---|
| MedCom OOG Type | (0029,xx08) | SIEMENS MEDCOM OOG | 1 | MEDCOM Object Oriented Graphics (OOG) identification characteristics.<br>Defined Terms:<br>MEDCOM OOG 1<br>MEDCOM OOG 2 |
| MedCom OOG Version | (0029,xx09) | SIEMENS MEDCOM OOG | 3 | Version of MEDCOM OOG Info (0029,xx10) format. |
| MedCom OOG Info | (0029,xx10) | SIEMENS MEDCOM OOG | 3 | MEDCOM Object Oriented Graphics (OOG) data. |

Table 78 MEDCOM OOG Module

The graphics objects are also fully drawn in the Image Overlay Plane for compatibility with other products, which do not support the MedCom OOG module. Any system not supporting the MedCom OOG module shall remove the OOG module and its content when modifying the image overlay plane content.

### A.2.3 Edge Enhancement Module

The table in this section contains private IOD Attributes that describe Edge Enhancement extensions due to the Dynamic Cardio Review definition.

| Attribute Name | Tag | Owner | Type | Notes |
|---|---|---|---|---|
| Standard Edge Enhancement Sequence | (0029,xx00) | CARDIO-D.R. 1.0 | 3 | Standard formula according to Dyna view Extensions. |
| >Convolution Kernel Size | (0029,xx01) | CARDIO-D.R. 1.0 | 1C | x-/y-size value pair.<br>Each value shall be greater or equal to 3.<br><br>Required if sequence is present |
| >Convolution Kernel Coefficients | (0029,xx02) | CARDIO-D.R. 1.0 | 1C | Row-by-row list of the kernel Coefficients.<br><br>Required if sequence is present |
| >Edge Enhancement Gain | (0029,xx03) | CARDIO-D.R. 1.0 | 1C | Applied Filter gain Factor. Range is from 0 to 100 Percent.<br><br>Required if sequence is present |

Table 79 Edge Enhancement Module

### A.2.4 Angio Viewing Module

The table in this section contains private IOD Attributes that describe additional Attributes for advanced Angio Viewing features

| Attribute Name | Tag | Owner | Type | Notes |
|---|---|---|---|---|
| Review Mode | (0019,xx00) | SIEMENS SMS-AX VIEW 1.0 | 3 | Special Modes for Angio Review.<br>Defined Terms are<br>1 = REV_MAXFILL,<br>2 = REV_LOOP,<br>3 = REV_SCROLL,<br>4 = REV_STEREO_LOOP |
| Anatomical Background Percent | (0019,xx01) | SIEMENS SMS-AX VIEW 1.0 | 3 | Percentage of Mix between Subtracted Image Result and Native Mask. Range is from 0 to 100. |
| Number of Phases | (0019,xx02) | SIEMENS SMS-AX VIEW 1.0 | 3 | 1-4 (1 or # of “Variable Frame Rate” acq phases) |
| Apply Anatomical Background | (0019,xx03) | SIEMENS SMS-AX VIEW 1.0 | 3 | Boolean |
| Pixel Shift Array | (0019,xx04) | SIEMENS SMS-AX VIEW 1.0 | 3 | 4 * Number of Frames (0028,0008) |
| Brightness | (0019,xx05) | SIEMENS SMS-AX VIEW 1.0 | 3 | SUB windowing |
| Contrast | (0019,xx06) | SIEMENS SMS-AX VIEW 1.0 | 3 | SUB windowing |
| Enabled Shutter | (0019,xx07) | SIEMENS SMS-AX VIEW 1.0 | 3 | Visualize shutter |
| Native Edge Enhancement Percent Gain | (0019,xx08) | SIEMENS SMS-AX VIEW 1.0 | 3 | Percent gain for native display of images. |
| Native Edge Enhancement LUT Index | (0019,xx09) | SIEMENS SMS-AX VIEW 1.0 | 3 | |
| Native Edge Enhancement Kernel Size | (0019,xx0A) | SIEMENS SMS-AX VIEW 1.0 | 3 | |
| Subtracted Edge Enhancement Percent Gain | (0019,xx0B) | SIEMENS SMS-AX VIEW 1.0 | 3 | Percent gain for subtracted display of images. |
| Subtracted Edge Enhancement LUT Index | (0019,xx0C) | SIEMENS SMS-AX VIEW 1.0 | 3 | |
| Subtracted Edge Enhancement Kernel Size | (0019,xx0D) | SIEMENS SMS-AX VIEW 1.0 | 3 | |

| Attribute Name | Tag | Owner | Type | Notes |
|---|---|---|---|---|
| Fade Percent | (0019,xx0E) | SIEMENS SMS-AX VIEW 1.0 | 3 | |
| Flipped before Laterality Applied | (0019,xx0F) | SIEMENS SMS-AX VIEW 1.0 | 3 | |
| Apply Fade | (0019,xx10) | SIEMENS SMS-AX VIEW 1.0 | 3 | |
| Zoom | (0019,xx12) | SIEMENS SMS-AX VIEW 1.0 | 3 | |
| Pan X | (0019,xx13) | SIEMENS SMS-AX VIEW 1.0 | 3 | |
| Pan Y | (0019,xx14) | SIEMENS SMS-AX VIEW 1.0 | 3 | |
| Native Edge Enhancement Adverse Percent Gain | (0019,xx15) | SIEMENS SMS-AX VIEW 1.0 | 3 | |
| Subtracted Edge Enhancement Adverse Percent Gain | (0019,xx16) | SIEMENS SMS-AX VIEW 1.0 | 3 | |
| Invert Flag | (0019,xx17) | SIEMENS SMS-AX VIEW 1.0 | 3 | |
| Quant 1K Overlay | (0019,xx1A) | SIEMENS SMS-AX VIEW 1.0 | 3 | Only Store Monitor and Store Reference Images in Quant (128 kbyte) |
| Original Resolution | (0019,xx1B) | SIEMENS SMS-AX VIEW 1.0 | 3 | internal usage only |
| Auto Window Center | (0019,xx1C) | SIEMENS SMS-AX VIEW 1.0 | 3 | |
| Auto Window Width | (0019,xx1D) | SIEMENS SMS-AX VIEW 1.0 | 3 | |
| Auto Window Correct Value | (0019,xx1E) | SIEMENS SMS-AX VIEW 1.0 | 3 | |

Table 80 Angio Viewing Module

## A.2.5 Angio Acquisition Data Module

The table in this section contains private IOD Attributes that describe additional Attributes for saving specific Angio Acquisition data.

| Attribute Name | Tag | Owner | Type | Notes |
|---|---|---|---|---|
| Acquisition Type | (0021,xx00) | SIEMENS SMS-AX ACQ 1.0 | 3 | Technical Type of Acquisition performed to get image result.<br>Defined Terms are<br>1 = fixed frame rate,<br>2 = variable frame rate (manually triggered),<br>3 = variable frame rate (time triggered),<br>4 = peri manual to head,<br>10 = dynavision manual inject.,<br>11 = dynavision automatic,<br>14 = pulsed fluoro,<br>15 = ECG triggered fluoro<br>16 = scanning slow speed<br>17 = scanning fast speed |

| Attribute Name | Tag | Owner | Type | Notes |
|---|---|---|---|---|
| Acquisition Mode | (0021,xx01) | SIEMENS SMS-AX ACQ 1.0 | 3 | Technical Mode of Acquisition performed<br>to get image result.<br>Defined Terms are:<br>0 = no mode specified,<br>1 = Digital Radiography,<br>2 = DSA,<br>3 = Peri-DSA,<br>4 = DR stepping,<br>5 = DR Dynavision (nat),<br>6 = Dynavision (sub),<br>7 = Card,<br>9 = 3D Mode<br>20 = Roadmap Fluoro,<br>21 = Normal Fluoro,<br>22 = Card Fluoro |
| Foot Switch Index | (0021,xx02) | SIEMENS SMS-AX ACQ 1.0 | 3 | |
| Acquisition Room | (0021,xx03) | SIEMENS SMS-AX ACQ 1.0 | 3 | |
| Current Time Product | (0021,xx04) | SIEMENS SMS-AX ACQ 1.0 | 3 | (uAs) |
| Dose | (0021,xx05) | SIEMENS SMS-AX ACQ 1.0 | 3 | (uGy/pulse) |
| Skin Dose Percent | (0021,xx06) | SIEMENS SMS-AX ACQ 1.0 | 3 | |
| Skin Dose Accumulation | (0021,xx07) | SIEMENS SMS-AX ACQ 1.0 | 3 | mGy |
| Skin Dose Rate | (0021,xx08) | SIEMENS SMS-AX ACQ 1.0 | 3 | Percent gain for native display of images. |
| Copper Filter | (0021,xx0A) | SIEMENS SMS-AX ACQ 1.0 | 3 | |
| Measuring Field | (0021,xx0B) | SIEMENS SMS-AX ACQ 1.0 | 3 | Decimal values are defined as follows:<br>1 = left<br>2 = middle (rectangular)<br>3 = left and middle<br>4 = right<br>5 = left and right<br>6 = right and middle<br>7 = left and right and middle<br>8 = central (approx. round)<br>9 = left and central<br>12 = right and central<br>13 = left and right and central |
| Total Steps | (0021,xx0E) | SIEMENS SMS-AX ACQ 1.0 | 3 | Number of Images which make up a Peri or DR-Step acquisition |
| Dyna X-Ray Info | (0021,xx0F) | SIEMENS SMS-AX ACQ 1.0 | 3 | Multiplicity of (4 * Number of Frames).<br>(kV value, uA value, ms, uAs value)<br>Only with Dyna Images |
| Gamma Input | (0021,xx10) | SIEMENS SMS-AX ACQ 1.0 | 3 | |
| Gamma Output | (0021,xx11) | SIEMENS SMS-AX ACQ 1.0 | 3 | |
| SH_STPAR | (0021,xx12) | SIEMENS SMS-AX ACQ 1.0 | 3 | 1st Byte = version. Technical data-structure with Gantry information. |
| Acquisition Zoom | (0021,xx13) | SIEMENS SMS-AX ACQ 1.0 | 3 | 0 = Off, 1 = On.<br>Not to be mixed up with digital zoom from Viewing module. |
| DDO Value | (0021,xx15) | SIEMENS SMS-AX ACQ 1.0 | 3 | |
| DR Single Flag | (0021,xx16) | SIEMENS SMS-AX ACQ 1.0 | 3 | 1 = DR SINGLE, else single Frame DR acquisition |
| Source to Isocenter | (0021,xx17) | SIEMENS SMS-AX ACQ 1.0 | 3 | (mm) |
| ECG Index Array | (0021,xx19) | SIEMENS SMS-AX ACQ 1.0 | 3 | |
| FD Flag | (0021,xx1A) | SIEMENS SMS-AX ACQ 1.0 | 3 | |

| Attribute Name | Tag | Owner | Type | Notes |
|---|---|---|---|---|
| SH_ZOOM | (0021,xx1B) | SIEMENS SMS-AX ACQ 1.0 | 3 | |
| SH_COLPAR | (0021,xx1C) | SIEMENS SMS-AX ACQ 1.0 | 3 | 1st Byte = version. Technical data-structure with collimator information. |
| K-Factor | (0021,xx1D) | SIEMENS SMS-AX ACQ 1.0 | 3 | |
| EVE | (0021,xx1E) | SIEMENS SMS-AX ACQ 1.0 | 3 | |
| Total Scene Time | (0021,xx1F) | SIEMENS SMS-AX ACQ 1.0 | 3 | |
| Restore Flag | (0021,xx20) | SIEMENS SMS-AX ACQ 1.0 | 3 | |
| Stand Movement Flag | (0021,xx21) | SIEMENS SMS-AX ACQ 1.0 | 3 | |
| FD Rows | (0021,xx22) | SIEMENS SMS-AX ACQ 1.0 | 3 | Acquisition matrix, rows |
| FD Columns | (0021,xx23) | SIEMENS SMS-AX ACQ 1.0 | 3 | Acquisition matrix, columns |
| Table Movement Flag | (0021,xx24) | SIEMENS SMS-AX ACQ 1.0 | 3 | |
| Crispy XPI Filter | (0021,xx26) | SIEMENS SMS-AX ACQ 1.0 | 3 | |
| IC Stent Flag | (0021,xx27) | SIEMENS SMS-AX ACQ 1.0 | 3 | |
| Gamma LUT Sequence | (0021,xx28) | SIEMENS SMS-AX ACQ 1.0 | 3 | |
| 3D Cardiac Phase Center | (0021,xx2A) | SIEMENS SMS-AX ACQ 1.0 | 3 | |
| 3D Cardiac Phase Width | (0021,xx2B) | SIEMENS SMS-AX ACQ 1.0 | 3 | |
| Organ Program Info | (0021,xx30) | SIEMENS SMS-AX ACQ 1.0 | 3 | 1st Byte = version. Technical data-structure with organ program information |
| mAs Modulation | (0021,xx3B) | SIEMENS SMS-AX ACQ 1.0 | 3 | only for cardiac triggered 3D acquisition |
| 3D R-Peak Reference Time | (0021,xx3C) | SIEMENS SMS-AX ACQ 1.0 | 3 | only for cardiac triggered 3D acquisition |
| Gamma LUT Descriptor | (0021,xx40) | SIEMENS SMS-AX ACQ 1.0 | 3 | |
| Gamma LUT Type | (0021,xx41) | SIEMENS SMS-AX ACQ 1.0 | 3 | |
| Gamma LUT Data | (0021,xx42) | SIEMENS SMS-AX ACQ 1.0 | 3 | |
| 3D Cardiac Trigger Sequence | (0021,xxA3) | SIEMENS SMS-AX ACQ 1.0 | 3 | only for cardiac triggered 3D acquisition |
| 3D Frame Reference Date Time | (0021,xxA4) | SIEMENS SMS-AX ACQ 1.0 | 3 | only for cardiac triggered 3D acquisition |
| 3D Cardiac Trigger Delay Time | (0021,xxA5) | SIEMENS SMS-AX ACQ 1.0 | 3 | only for cardiac triggered 3D acquisition |
| 3D R-R Interval Time Measured | (0021,xxA6) | SIEMENS SMS-AX ACQ 1.0 | 3 | only for cardiac triggered 3D acquisition |

Table 81 Angio Acquisition Data Module

### A.2.6 Angio Quantification Module

The table in this section contains private IOD Attributes that describe additional Attributes for advanced Angio Quantification and Calibration Results features

| Attribute Name | Tag | Owner | Type | Notes |
|---|---|---|---|---|
| Calibration TOD Value | (0023,xx08) | SIEMENS SMS-AX QUANT 1.0 | 3 | |
| Calibration Method | (2121,xx01) | PMI Private Calibration Module Version 2.0 | 3 | only for Quant Reports |

| | | | | |
|---|---|---|---|---|
| Calibration Method Info | (2121,xx02) | PMI Private Calibration Module Version 2.0 | 3 | only for Quant Reports |
| Calibration Object Size | (2121,xx03) | PMI Private Calibration Module Version 2.0 | 3 | only for Quant Reports |
| Calibration Object S Dev | (2121,xx04) | PMI Private Calibration Module Version 2.0 | 3 | only for Quant Reports |
| Calibration Horizontal Pixel Spacing | (2121,xx05) | PMI Private Calibration Module Version 2.0 | 3 | only for Quant Reports |
| Calibration Vertical Pixel Spacing | (2121,xx06) | PMI Private Calibration Module Version 2.0 | 3 | only for Quant Reports |
| Calibration File Name | (2121,xx07) | PMI Private Calibration Module Version 2.0 | 3 | only for Quant Reports |
| Calibration Frame Number | (2121,xx08) | PMI Private Calibration Module Version 2.0 | 3 | only for Quant Reports |
| Calibration Object Unit | (2121,xx09) | PMI Private Calibration Module Version 2.0 | 3 | only for Quant Reports |
| Averaged Calibrations Performed | (2121,xx0A) | PMI Private Calibration Module Version 2.0 | 3 | only for Quant Reports |
| Auto Magnify Factor | (2121,xx0B) | PMI Private Calibration Module Version 2.0 | 3 | only for Quant Reports |
| Horizontal Pixel S Dev | (2121,xx0C) | PMI Private Calibration Module Version 2.0 | 3 | only for Quant Reports |
| Vertical Pixel S Dev | (2121,xx0D) | PMI Private Calibration Module Version 2.0 | 3 | only for Quant Reports |
| Calibration Method | (2121,xx0E) | PMI Private Calibration Module Version 2.0 | 3 | only for Quant Reports |

Table 82 Angio Quantification Module

### A.2.7 Original Image Info Module

The table in this section contains private IOD Attributes that describe additional original image data for derived images (e.g. Store Monitor Image).

| Attribute Name | Tag | Owner | Type | Notes |
|---|---|---|---|---|
| View Native | (0025,xx00) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | 3 | |
| Original Series Number | (0025,xx01) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | 3 | |
| Original Image Number | (0025,xx02) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | 3 | |
| Win Center | (0025,xx03) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | 3 | |
| Win Width | (0025,xx04) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | 3 | |
| Win Brightness | (0025,xx05) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | 3 | |
| Win Contrast | (0025,xx06) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | 3 | |
| Original Frame Number | (0025,xx07) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | 3 | |
| Original Mask Frame Number | (0025,xx08) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | 3 | |
| Opac | (0025,xx09) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | 3 | |
| Original Number of Frames | (0025,xx0A) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | 3 | |
| Original Scene Duration | (0025,xx0B) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | 3 | |
| Identifier LOID | (0025,xx0C) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | 3 | Set to "AXIM_READY_PROCESSED" when Ready Processing was applied |
| Original Scene VFR Info | (0025,xx0D) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | 3 | Number of phases, then followed by n pairs (Last Frame Number, then Frame Rate) |
| Original Frame ECG Position | (0025,xx0E) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | 3 | |
| Original ECG 1st Frame Offset | (0025,xx0F) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | 3 | <retired, no longer used> |
| Zoom Flag | (0025,xx10) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | 3 | |
| Flex | (0025,xx11) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | 3 | |
| Number of Mask Frames | (0025,xx12) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | 3 | |
| Number of Fill Frames | (0025,xx13) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | 3 | |
| Series Number | (0025,xx14) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | 3 | |
| Image Number | (0025,xx15) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | 3 | |

Table 83 Original Image Info Module

### A.2.8 SOP Common Module – Image Type Extensions

Additional values for the image type attribute are used to designate the purpose of the SOP instance created by the Artis zee VC13 system. Please see the following table for details.

| Type of Scene/Image | Image Type |
|---|---|
| Single Plane Scene | ORIGINAL\PRIMARY\SINGLE PLANE\SINGLE A (or B) |
| Biplane Scene | ORIGINAL\PRIMARY\BIPLANE A (or B) |
| Reference Image | DERIVED\SECONDARY\SINGLE PLANE\SINGLE A(B)\REFIMAGE |
| Reference Image from CT | DERIVED\SECONDARY\SINGLE PLANE\SINGLE A\REFIMAGE\CT REF |
| Reference Image from MR | DERIVED\SECONDARY\SINGLE PLANE\SINGLE A\REFIMAGE\MR REF |
| Dynamic Reference Image (Dynamap) | DERIVED\SECONDARY\SINGLE PLANE\SINGLE A(B)\DYNAMAP |
| Store Monitor | DERIVED\SECONDARY\SINGLE PLANE\SINGLE A(B)\STORE MONITOR |
| Secondary Capture | DERIVED\SECONDARY\SINGLE PLANE\PLANE A(B)\SC |
| Perivision - Mask Phase | ORIGINAL\PRIMARY\SINGLE PLANE\PLANE A\PERI\MASK\n[1] |
| Perivision - Fill Phase | ORIGINAL\PRIMARY\SINGLE PLANE\PLANE A\PERI\FILL\n[1] |
| Dynavision - Mask Phase | ORIGINAL\PRIMARY\SINGLE PLANE\PLANE A\DYNA\MASK |
| Dynavision - Fill Phase | ORIGINAL\PRIMARY\SINGLE PLANE\PLANE A\DYNA\FILL |
| Dynavision - Injection Phase | ORIGINAL\PRIMARY\SINGLE PLANE\PLANE A\DYNA\INJECTION |
| Dynavision - Washout Phase | ORIGINAL\PRIMARY\SINGLE PLANE\PLANE A\DYNA\WASHOUT |
| 3D Acquisition DR | ORIGINAL\PRIMARY\SINGLE PLANE\SINGL A(B)\3D ACQ\DR[2] |
| 3D Acquisition DSA | ORIGINAL\PRIMARY\SINGLE PLANE\SINGL A(B)\3D ACQ\DSA[2] |
| 3D Acquisition CARD | ORIGINAL\PRIMARY\SINGLE PLANE\SINGL A(B)\3D ACQ\CARD[2] |
| Store Fluoro Loop | DERIVED\PRIMARY\SINGLE PLANE\SINGLE A(or B)\STORE FLUORO |
| Store Biplane Fluoro Loop | DERIVED\PRIMARY\BIPLANE A(or B)\\STORE FLUORO |
| Quant Result Image | DERIVED\SECONDARY\\<3rd to nth value from Original>\QUANT |
| Exam Protocol (Non-Image Object) | ORIGINAL\PRIMARY\SINGLE PLANE\\EXAM PROTOCOL |

[1] the term "n" is replaced by the related Step Number where the Image was acquired. Step Numbers start with "1".
[2] Additional values with phase info are set

Table 84 Image Type Extensions

## A.3 Registry of private DICOM Data Elements

| Tag | Private Owner Code | Name | VR | VM |
|---|---|---|---|---|
| (0019,xx00) | SIEMENS SMS-AX VIEW 1.0 | Review Mode | US | 1 |
| (0019,xx01) | SIEMENS SMS-AX VIEW 1.0 | Anatomical Background Percent | US | 1 |
| (0019,xx02) | SIEMENS SMS-AX VIEW 1.0 | Number of Phases | US | 1 |
| (0019,xx03) | SIEMENS SMS-AX VIEW 1.0 | Apply Anatomical Background | US | 1 |
| (0019,xx04) | SIEMENS SMS-AX VIEW 1.0 | Pixel Shift Array | SS | 4-4n |
| (0019,xx05) | SIEMENS SMS-AX VIEW 1.0 | Brightness | US | 1 |
| (0019,xx06) | SIEMENS SMS-AX VIEW 1.0 | Contrast | US | 1 |
| (0019,xx07) | SIEMENS SMS-AX VIEW 1.0 | Enabled | US | 1 |
| (0019,xx08) | SIEMENS SMS-AX VIEW 1.0 | Native Edge Enh. Percent Gain | US | 1 |
| (0019,xx09) | SIEMENS SMS-AX VIEW 1.0 | Native Edge Enh. LUT Index | SS | 1 |
| (0019,xx0A) | SIEMENS SMS-AX VIEW 1.0 | Native Edge Enh. Kernel Size | SS | 1 |
| (0019,xx0B) | SIEMENS SMS-AX VIEW 1.0 | Subtr. Edge Enh. Percent Gain | US | 1 |
| (0019,xx0C) | SIEMENS SMS-AX VIEW 1.0 | Subtr. Edge Enh. LUT Index | SS | 1 |
| (0019,xx0D) | SIEMENS SMS-AX VIEW 1.0 | Subtr. Edge Enh. Kernel Size | SS | 1 |
| (0019,xx0E) | SIEMENS SMS-AX VIEW 1.0 | Fade Percent | US | 1 |
| (0019,xx0F) | SIEMENS SMS-AX VIEW 1.0 | Flipped Before Laterality Applied | US | 1 |
| (0019,xx10) | SIEMENS SMS-AX VIEW 1.0 | Apply Fade | US | 1 |
| (0019,xx12) | SIEMENS SMS-AX VIEW 1.0 | Zoom | US | 1 |
| (0019,xx13) | SIEMENS SMS-AX VIEW 1.0 | Pan X | SS | 1 |
| (0019,xx14) | SIEMENS SMS-AX VIEW 1.0 | Pan Y | SS | 1 |
| (0019,xx15) | SIEMENS SMS-AX VIEW 1.0 | Native Edge Enh. Adv Perc. Gain | SS | 1 |
| (0019,xx16) | SIEMENS SMS-AX VIEW 1.0 | Subtr. Edge Enh. Adv Perc. Gain | SS | 1 |
| (0019,xx17) | SIEMENS SMS-AX VIEW 1.0 | Invert Flag | US | 1 |
| (0019,xx1A) | SIEMENS SMS-AX VIEW 1.0 | Quant 1K Overlay | OB | 1 |
| (0019,xx1B) | SIEMENS SMS-AX VIEW 1.0 | Original Resolution | US | 1 |
| (0019,xx1C) | SIEMENS SMS-AX VIEW 1.0 | Auto Window Center | DS | 1 |
| (0019,xx1D) | SIEMENS SMS-AX VIEW 1.0 | Auto Window Width | DS | 1 |
| (0019,xx1E) | SIEMENS SMS-AX VIEW 1.0 | Auto Window Correct Value | IS | 2 |

Table 85 Private Elements in Group 0019

| Tag | Private Owner Code | Name | VR | VM |
|---|---|---|---|---|
| (0021,xx00) | SIEMENS SMS-AX ACQ 1.0 | Acquisition Type | US | 1 |
| (0021,xx01) | SIEMENS SMS-AX ACQ 1.0 | Acquisition Mode | US | 1 |
| (0021,xx02) | SIEMENS SMS-AX ACQ 1.0 | Footswitch Index | US | 1 |
| (0021,xx03) | SIEMENS SMS-AX ACQ 1.0 | Acquisition Room | US | 1 |
| (0021,xx04) | SIEMENS SMS-AX ACQ 1.0 | Current Time Product | SL | 1 |
| (0021,xx05) | SIEMENS SMS-AX ACQ 1.0 | Dose | SL | 1 |
| (0021,xx06) | SIEMENS SMS-AX ACQ 1.0 | Skin Dose Percent | SL | 1 |
| (0021,xx07) | SIEMENS SMS-AX ACQ 1.0 | Skin Dose Accumulation | SL | 1 |
| (0021,xx08) | SIEMENS SMS-AX ACQ 1.0 | Skin Dose Rate | SL | 1 |
| (0021,xx0A) | SIEMENS SMS-AX ACQ 1.0 | Copper Filter | UL | 1 |
| (0021,xx0B) | SIEMENS SMS-AX ACQ 1.0 | Measuring Field | US | 1 |
| (0021,xx0E) | SIEMENS SMS-AX ACQ 1.0 | Total Steps | SS | 1 |
| (0021,xx0F) | SIEMENS SMS-AX ACQ 1.0 | Dyna X-Ray Info | SL | 3-3n |
| (0021,xx10) | SIEMENS SMS-AX ACQ 1.0 | Modality LUT Input Gamma | ÚS | 1 |
| (0021,xx11) | SIEMENS SMS-AX ACQ 1.0 | Modality LUT Output Gamma | US | 1 |
| (0021,xx12) | SIEMENS SMS-AX ACQ 1.0 | SH_STPAR | OB | 1-n |
| (0021,xx13) | SIEMENS SMS-AX ACQ 1.0 | Acquisition Zoom | US | 1 |
| (0021,xx15) | SIEMENS SMS-AX ACQ 1.0 | DDO Value | US | 1 |

| Tag | Private Owner Code | Name | VR | VM |
|---|---|---|---|---|
| (0021,xx16) | SIEMENS SMS-AX ACQ 1.0 | DR Single Flag | US | 1 |
| (0021,xx17) | SIEMENS SMS-AX ACQ 1.0 | Source to Isocenter | SL | 1 |
| (0021,xx19) | SIEMENS SMS-AX ACQ 1.0 | ECG Index Array | SL | 1 |
| (0021,xx1A) | SIEMENS SMS-AX ACQ 1.0 | FD Flag | US | 1 |
| (0021,xx1B) | SIEMENS SMS-AX ACQ 1.0 | SH_ZOOM | OB | 1 |
| (0021,xx1C) | SIEMENS SMS-AX ACQ 1.0 | SH_COLPAR | OB | 1 |
| (0021,xx1D) | SIEMENS SMS-AX ACQ 1.0 | K-Factor | US | 1 |
| (0021,xx1E) | SIEMENS SMS-AX ACQ 1.0 | EVE | US | 8 |
| (0021,xx1F) | SIEMENS SMS-AX ACQ 1.0 | Total Scene Time | SL | 1 |
| (0021,xx20) | SIEMENS SMS-AX ACQ 1.0 | Restore Flag | US | 1 |
| (0021,xx21) | SIEMENS SMS-AX ACQ 1.0 | Stand Movement Flag | US | 1 |
| (0021,xx22) | SIEMENS SMS-AX ACQ 1.0 | FD Rows | US | 1 |
| (0021,xx23) | SIEMENS SMS-AX ACQ 1.0 | FD Columns | US | 1 |
| (0021,xx24) | SIEMENS SMS-AX ACQ 1.0 | Table Movement Flag | US | 1 |
| (0021,xx26) | SIEMENS SMS-AX ACQ 1.0 | Crispy XPI Filter | DS | 1 |
| (0021,xx27) | SIEMENS SMS-AX ACQ 1.0 | IC Stent Flag | US | 1 |
| (0021,xx28) | SIEMENS SMS-AX ACQ 1.0 | Gamma LUT Sequence | SQ | 1 |
| (0021,xx2A) | SIEMENS SMS-AX ACQ 1.0 | 3D Cardiac Phase Center | IS | 1 |
| (0021,xx2B) | SIEMENS SMS-AX ACQ 1.0 | 3D Cardiac Phase Width | IS | 1 |
| (0021,xx30) | SIEMENS SMS-AX ACQ 1.0 | Organ Program Info | OB | 1 |
| (0021,xx3B) | SIEMENS SMS-AX ACQ 1.0 | mAs Modulation | IS | 1 |
| (0021,xx3C) | SIEMENS SMS-AX ACQ 1.0 | 3D R-Peak Reference Time | DT | 1-n |
| (0021,xx40) | SIEMENS SMS-AX ACQ 1.0 | Gamma LUT Descriptor | US | 3 |
| (0021,xx41) | SIEMENS SMS-AX ACQ 1.0 | Gamma LUT Type | LO | 1 |
| (0021,xx42) | SIEMENS SMS-AX ACQ 1.0 | Gamma LUT Data | US | 1-n |
| (0021,xxA3) | SIEMENS SMS-AX ACQ 1.0 | 3D Cardiac Trigger Sequence | SQ | 1 |
| (0021,xxA4) | SIEMENS SMS-AX ACQ 1.0 | 3D Frame Reference Date Time | DT | 1 |
| (0021,xxA5) | SIEMENS SMS-AX ACQ 1.0 | 3D Cardiac Trigger Delay Time | FD | 1 |
| (0021,xxA6) | SIEMENS SMS-AX ACQ 1.0 | 3D R-R Interval Time Measured | FD | 1 |

Table 86 Private Elements in Group 0021

| Tag | Private Owner Code | Name | VR | VM |
|---|---|---|---|---|
| (0023,xx08) | SIEMENS SMS-AX QUANT 1.0 | Calibration TOD Value | IS | 1 |

Table 87 Private Elements in Group 0023

| Tag | Private Owner Code | Name | VR | VM |
|---|---|---|---|---|
| (0025,xx00) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | View Native | US | 1 |
| (0025,xx01) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | Original Series Number | US | 1 |
| (0025,xx02) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | Original Image Number | US | 1 |
| (0025,xx03) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | Win Center | US | 1 |
| (0025,xx04) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | Win Width | US | 1 |
| (0025,xx05) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | Win Brightness | US | 1 |
| (0025,xx06) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | Win Contrast | US | 1 |
| (0025,xx07) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | Original Frame Number | US | 1 |
| (0025,xx08) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | Original Mask Frame Number | US | 1 |
| (0025,xx09) | SIEMENS SMS-AX ORIGINAL | Opac | US | 1 |

| Tag | Private Owner Code | Name | VR | VM |
|---|---|---|---|---|
| | IMAGE INFO 1.0 | | | |
| (0025,xx0A) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | Original Number of Frames | US | 1 |
| (0025,xx0B) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | Original Scene Duration | DS | 1 |
| (0025,xx0C) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | Identifier LOID | LO | 1 |
| (0025,xx0D) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | Original Scene VFR Info | SS | 1-n |
| (0025,xx0E) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | Original Frame ECG Position | SS | 1 |
| (0025,xx0F) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | Original ECG 1st Frame Offset(retired) | SS | 1 |
| (0025,xx10) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | Zoom Flag | SS | 1 |
| (0025,xx11) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | Flexible Pixel Shift | US | 1 |
| (0025,xx12) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | Number of Mask Frames | US | 1 |
| (0025,xx13) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | Number of Fill Frames | US | 1 |
| (0025,xx14) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | Series Number | IS | 1 |
| (0025,xx15) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 | Image Number | IS | 1 |

Table 88 Private Elements in Group 0025

| Tag | Private Owner Code | Name | VR | VM |
|---|---|---|---|---|
| (0029,xx08) | SIEMENS CSA NON-IMAGE | CSA Data Type | CS | 1 |
| (0029,xx09) | SIEMENS CSA NON-IMAGE | CSA Data Version | LO | 1 |
| (0029,xx10) | SIEMENS CSA NON-IMAGE | CSA Data Info | OB | 1 |
| (0029,xx08) | SIEMENS MEDCOM HEADER | MedCom Header Type | CS | 1 |
| (0029,xx09) | SIEMENS MEDCOM HEADER | MedCom Header Version | LO | 1 |
| (0029,xx10) | SIEMENS MEDCOM HEADER | MedCom Header Info | OB | 1 |
| (0029,xx20) | SIEMENS MEDCOM HEADER | MedCom History Information | OB | 1 |
| (0029,xx31) | SIEMENS MEDCOM HEADER | PMTF Information 1 | LO | 1 |
| (0029,xx32) | SIEMENS MEDCOM HEADER | PMTF Information 2 | UL | 1 |
| (0029,xx33) | SIEMENS MEDCOM HEADER | PMTF Information 3 | UL | 1 |
| (0029,xx34) | SIEMENS MEDCOM HEADER | PMTF Information 4 | CS | 1 |
| (0029,xx35) | SIEMENS MEDCOM HEADER | PMTF Information 5 | UL | 1 |
| (0029,xx40) | SIEMENS MEDCOM HEADER | Application Header Sequence | SQ | 1 |
| (0029,xx41) | SIEMENS MEDCOM HEADER | Application Header Type | CS | 1 |
| (0029,xx42) | SIEMENS MEDCOM HEADER | Application Header ID | LO | 1 |
| (0029,xx43) | SIEMENS MEDCOM HEADER | Application Header Version | LO | 1 |
| (0029,xx44) | SIEMENS MEDCOM HEADER | Application Header Info | OB | 1 |
| (0029,xx50) | SIEMENS MEDCOM HEADER | Workflow Control Flags | LO | 8 |
| (0029,xx51) | SIEMENS MEDCOM HEADER | Arch. Management Flag Keep Online | CS | 1 |
| (0029,xx52) | SIEMENS MEDCOM HEADER | Arch. Mgmnt Flag Do Not Archive | CS | 1 |
| (0029,xx53) | SIEMENS MEDCOM HEADER | Image Location Status | CS | 1 |
| (0029,xx54) | SIEMENS MEDCOM HEADER | Estimated Retrieve Time | DS | 1 |
| (0029,xx55) | SIEMENS MEDCOM HEADER | Data Size of Retrieved Images | DS | 1 |
| (0029,xx60) | SIEMENS MEDCOM HEADER2 | Series Workflow Status | LO | 1 |
| (0029,xx08) | SIEMENS MEDCOM OOG | MedCom OOG Type | CS | 1 |
| (0029,xx09) | SIEMENS MEDCOM OOG | MedCom OOG Version | LO | 1 |
| (0029,xx10) | SIEMENS MEDCOM OOG | MedCom OOG Info | OB | 1 |
| (0029,xx00) | CARDIO-D.R. 1.0 | Standard Edge Enhancement Sequence | SQ | 1 |
| (0029,xx01) | CARDIO-D.R. 1.0 | Convolution Kernel Size | US | 2 |

| | | | | |
|---|---|---|---|---|
| (0029,xx02) | CARDIO-D.R. 1.0 | Convolution Kernel Coefficients | US | 1-n |
| (0029,xx03) | CARDIO-D.R. 1.0 | Edge Enhancement Gain | FL | 1 |
| (7FE1,xx10) | SIEMENS CSA NON-IMAGE | CSA Data | OB | 1 |

Table 89 Private Elements in Group 0029 and 7FE1

| Tag | Private Owner Code | Name | VR | VM |
|---|---|---|---|---|
| (2121,xx01) | PMI Private Calibration Module Version 2.0 | Calibration Method | ST | 1 |
| (2121,xx02) | PMI Private Calibration Module Version 2.0 | Calibration Method Info | ST | 1 |
| (2121,xx03) | PMI Private Calibration Module Version 2.0 | Calibration Object Size | FL | 1 |
| (2121,xx04) | PMI Private Calibration Module Version 2.0 | Calibration Object S Dev | FL | 1 |
| (2121,xx05) | PMI Private Calibration Module Version 2.0 | Calibration Horizontal Pixel Spacing | FL | 1 |
| (2121,xx06) | PMI Private Calibration Module Version 2.0 | Calibration Vertical Pixel Spacing | FL | 1 |
| (2121,xx08) | PMI Private Calibration Module Version 2.0 | Calibration File Name | ST | 1 |
| (2121,xx09) | PMI Private Calibration Module Version 2.0 | Calibration Frame Number | IS | 1 |
| (2121,xx0A) | PMI Private Calibration Module Version 2.0 | Calibration Object Unit | SH | 1 |
| (2121,xx0B) | PMI Private Calibration Module Version 2.0 | Averaged Calibrations Performed | SS | 1 |
| (2121,xx0C) | PMI Private Calibration Module Version 2.0 | Auto Magnify Factor | FL | 1 |
| (2121,xx0D) | PMI Private Calibration Module Version 2.0 | Horizontal Pixel S Dev | FL | 1 |
| (2121,xx0E) | PMI Private Calibration Module Version 2.0 | Vertical Pixel S Dev | FL | 1 |

Table 90 Private Elements in Group 2121

**Note**

Please be informed that some of the Private Owner Codes contain double-spaces in the name definitions. The following terms (only double-spaces marked) are defined:

SIEMENS SMS-AX<spc><spc>VIEW 1.0, SIEMENS SMS-AX<spc><spc>ACQ 1.0,

SIEMENS SMS-AX<spc><spc>QUANT 1.0, SIEMENS SMS-AX<spc><spc>ORIGINAL IMAGE INFO 1.0 All spaces not specially marked, are single spaces.

## A.4 Extended XA IOD

The Artis zee VC13 system will create images during acquisition and with post processing applications. Those will be encoded as XA Standard Extended SOP Class. Images created during post processing will be marked as derived. Please see the following table for a complete overview of supplied Type 1/2/3 Standard and additional Private Attributes:

The Standard DICOM Modules will be used to encode ECG data.

| Attribute Name | Tag | Value |
|---|---|---|
| Specific Character Set | (0008,0005) | From Configuration |
| Image Type | (0008,0008) | See “A.2.10. SOP Common Module-Image Type Extensions” |
| SOP Class UID | (0008,0016) | 1.2.840.10008.5.1.4.1.1.12.1 |
| SOP Instance UID | (0008,0018) | |
| Study Date | (0008,0020) | <yyyymmdd> |
| Series Date | (0008,0021) | <yyyymmdd> |
| Acquisition Date | (0008,0022) | Original: same as Content Date<br>Derived: Date of Original Acquisition |
| Content Date | (0008,0023) | <yyyymmdd> (Date of Creation) |
| Study Time | (0008,0030) | <hhmmss> |
| Series Time | (0008,0031) | <hhmmss> |
| Acquisition Time | (0008,0032) | Time of Original Acquisition |
| Content Time | (0008,0033) | <hhmmss> (Time of Creation) |
| Accession Number | (0008,0050) | RIS or “Accession No.” input |
| Modality | (0008,0060) | XA |
| Manufacturer | (0008,0070) | Siemens |
| Institution Name | (0008,0080) | RIS or “Institution Name” input |
| Institution Address | (0008,0081) | RIS |
| Referring Physician's Name | (0008,0090) | RIS or input |
| Station Name | (0008,1010) | from Configuration |
| Study Description | (0008,1030) | “Study” input |
| Series Description | (0008,103E) | “Organ Program” name or one of : EXAM PROTOCOL, , QCA REPORT, LVA REPORT |
| Physicians of Record | (0008,1048) | From RIS (0040,1010) Names of Intended Recipients of Results |
| Performing Physician's Name | (0008,1050) | “Performing Physician 1”\”Performing Physician 2” input |
| Operator's Name | (0008,1070) | “Operator 1”\”Operator 2” input |
| Admitting Diagnosis Description | (0008,1080) | “Admitting Diagnosis” input |
| Manufacturer's Model Name | (0008,1090) | AXIOM-Artis |
| Referenced Study Sequence | (0008,1110) | From RIS |
| >Referenced SOP Class UID | (0008,1150) | |
| >Referenced SOP Instance UID | (0008,1155) | |
| Referenced Performed Procedure Step Sequence | (0008,1111) | Set when MPPS is configured |
| >Referenced SOP Class UID | (0008,1150) | |
| >Referenced SOP Instance UID | (0008,1155) | |
| Referenced Patient Sequence | (0008,1120) | From RIS |
| >Referenced SOP Class UID | (0008,1150) | |
| >Referenced SOP Instance UID | (0008,1155) | |
| Referenced Image Sequence | (0008,1140) | Reference to related Plane with BIPLANE A/B Instances |
| >Referenced SOP Class UID | (0008,1150) | |
| >Referenced SOP Instance UID | (0008,1155) | |
| Derivation Description | (0008,2111) | Notes about transformation steps |

| Attribute Name | Tag | Value |
|---|---|---|
| Start Trim | (0008,2142) | <1 st frame to display> |
| Stop Trim | (0008,2143) | <last frame to display> |
| Recomm. Display Frame Rate | (0008,2144) | (in f/s) |
| Patient's Name | (0010,0010) | RIS or "Patient Name" input |
| Patient ID | (0010,0020) | RIS or "Patient ID" input |
| Patient's Birth Date | (0010,0030) | RIS or checked "DoB" input |
| Patient's Sex | (0010,0040) | RIS or input (M or F or O/unknown) |
| Other Patient IDs | (0010,1000) | From RIS |
| Other Patient Names | (0010,1001) | From RIS |
| Patient's Age | (0010,1010) | Calculated from “DoB” input |
| Patient's Size | (0010,1020) | (in meters) |
| Patient‘s Weight | (0010,1030) | (in kilograms) |
| Patient’s Address | (0010,1040) | “Address” input |
| Military Rank | (0010,1080) | From RIS |
| Medical Alerts | (0010,2000) | From RIS |
| Contrast Allergies | (0010,2110) | From RIS |
| Ethnic Group | (0010,2160) | From RIS |
| Smoking Status | (0010,21A0) | From RIS |
| Additional Patient History | (0010,21B0) | From RIS |
| Pregnancy Status | (0010,21C0) | From RIS |
| Last Menstrual Date | (0010,21D0) | From RIS |
| Patient Comment | (0010,4000) | “Additional Info” input |
| Contrast/Bolus Agent | (0018,0010) | |
| Cine Rate | (0018,0040) | <acquired frame rate> |
| KVP | (0018,0060) | <peak KV used> (KV) |
| Device Serial Number | (0018,1000) | <modality serial number> |
| Software Version | (0018,1020) | |
| Protocol Name | (0018,1030) | “Organ Program” input |
| Contrast Bolus Ingredient | (0018,1048) | |
| Frame Time | (0018,1063) | (msec/frame) |
| Frame Time Vector | (0018,1065) | <number of Frame values>(msec) |
| Distance Source to Detector | (0018,1110) | (mm) |
| Distance Source to Patient | (0018,1111) | (mm) |
| Estimated Radiographic Magnification Factor | (0018,1114) | <Ratio of SID/SOD> |
| Exposure Time | (0018,1150) | <duration of x-Ray exposure>(msec) |
| X-Ray Tube Current | (0018,1151) | (mA) |
| Average Pulse Width | (0018,1154) | (msec) |
| Radiation Setting | (0018,1155) | SC \| GR |
| Radiation Mode | (0018,115A) | CONTINUOUS \| PULSED |
| Image and Fluoroscopy Area Dose Product | (0018,115E) | (dGy*cm*cm) |
| Intensifier Size | (0018,1162) | <(zoomed) diameter> (mm) |
| Imager Pixel Spacing | (0018,1164) | <row space, col space>(mm) |
| Focal Spot | (0018,1190) | DYNAMIC \| STATIC |
| Positioner Motion | (0018,1500) | (degrees); 0 with DYNAMIC |
| Positioner Primary Angle | (0018,1510) | (degrees); 0 with DYNAMIC |
| Positioner Secondary Angle | (0018,1511) | Only with DYNAMIC (absolute values) |
| Positioner Primary Angle Increment | (0018,1520) | Only with DYNAMIC (absolute values) |
| Positioner Secondary Angle Increment | (0018,1521) | RECTANGULAR and/or CIRCULAR and/or POLYGONAL |
| Shutter Shape | (0018,1600) | DYNAMIC \| STATIC |
| Shutter Left Vertical Edge | (0018,1602) | <column number left edge> |
| Shutter Right Vertical Edge | (0018,1604) | <column number right edge> |
| Shutter Upper Horizontal Edge | (0018,1606) | <row number upper edge> |
| Shutter Lower Horizontal Edge | (0018,1608) | <row number lower edge> |

| Attribute Name | Tag | Value |
|---|---|---|
| Center of Circular Shutter | (0018,1610) | <row number>,<column number> |
| Radius of Circular Shutter | (0018,1612) | <number of pixels in row direction> |
| Vertices of the Polygonal Shutter | (0018,1620) | <list of row/column coordinate pairs> |
| Collimator Shape | (0018,1700) | RECTANGULAR and/or CIRCULAR and/or POLYGONAL |
| Collimator Left Vertical Edge | (0018,1702) | <column number left edge> |
| Collimator Right Vertical Edge | (0018,1704) | <column number right edge> |
| Collimator Upper Horizontal Edge | (0018,1706) | <row number upper edge> |
| Collimator Lower Horizontal Edge | (0018,1708) | <row number lower edge> |
| Center of Circular Collimator | (0018,1710) | <row number>,<column number> |
| Radius of Circular Collimator | (0018,1712) | <number of pixels in row direction> |
| Vertices of the Polygonal Collimator | (0018,1720) | <list of row/column coordinate pairs> |
| Patient Position | (0018,5100) | Mandatory “Patient Position” input |
| Private Creator | (0019,00xx) | SIEMENS SMS-AX VIEW 1.0 |
| *Attributes according to "A.2.6 Angio Viewing Module"* | | |
| Study Instance UID | (0020,000D) | RIS or system generated |
| Series Instance UID | (0020,000E) | |
| Study ID | (0020,0010) | |
| Series Number | (0020,0011) | |
| Instance Number | (0020,0013) | |
| Patient Orientation | (0020,0020) | calculated from "Patient Position" input and from Gantry coordinate data. |
| Laterality | (0020,0060) | input via L or R marker annotation, else absent |
| Images in Acquisition | (0020,1002) | |
| Image Comments | (0020,4000) | Not encoded or "SM" or "REF" |
| Private Creator | (0021,00xx) | SIEMENS SMS-AX ACQ 1.0 |
| *Attributes according to "A.2.7 Angio Acquisition Data Module"* | | |
| Private Creator | (0023,00xx) | SIEMENS SMS-AX QUANT 1.0 |
| *Attributes according to "A.2.8 Angio Quantification Module" if image was calibrated* | | |
| Private Creator | (0025,00xx) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 |
| *Attributes according to "A.2.9 Original Image Info Module"* | | |
| Samples per Pixel | (0028,0002) | 1 |
| Photometric Interpretation | (0028,0004) | MONOCHROME2 |
| Number of Frames | (0028,0008) | |
| Frame Increment Pointer | (0028,0009) | (0018,1063) or (0018,1065) for VFR |
| Rows | (0028,0010) | Up to 2480 |
| Columns | (0028,0011) | Up to 2480 |
| Bits Allocated | (0028,0100) | 8 \| 16 |
| Bits Stored | (0028,0101) | 8 \| 12 \| 16 |
| High Bit | (0028,0102) | 7 \| 11 \| 15 |
| Pixel Representation | (0028,0103) | 0 |
| Pixel Intensity Relationship | (0028,0103) | LIN \| LOG \| DISP |
| Window Center | (0028,1050) | <NAT value> |
| Window Width | (0028,1051) | <NAT value> |
| Recommended Viewing Mode | (0028,1090) | SUB \| NAT |
| Lossy Image Compression | (0028,2110) | |
| Modality LUT sequence | (0028,3000) | (if [0028,1040] = LOG) |
| >LUT Descriptor | (0028,3002) | <num of LUT entries>, <first pixel val mapped>, <Entry bits alloc> |
| >Modality LUT Type | (0028,3004) | US |
| >LUT data | (0028,3006) | <array of data, accord. descriptor> |
| Representative Frame Number | (0028,6010) | <e.g. frame number of Icon Image> |
| Mask Subtraction Sequence | (0028,6100) | |
| >Mask Operation | (0028,6101) | AVG_SUB |

| Attribute Name | Tag | Value |
|---|---|---|
| >Mask Frame Number | (0028,6110) | (only for AVG_SUB) |
| Private Creator | (0029,00xx) | CARDIO-D.R. 1.0 |
| Standard Edge Enhancement Sequence | (0029,xx00) | (if applied) contains two items |
| >Private Creator | (0029,00xx) | CARDIO-D.R. 1.0 |
| >Convolution Kernel Size | (0029,xx01) | <value Pair x-,y-size> |
| >Convolution kernel Coefficients | (0029xx02) | <row by row, as specified by size> |
| >Edge Enhancement Gain | (0029,xx03) | (in %) |
| >Private Creator | (0029,00xx) | SIEMENS MEDCOM HEADER |
| *Attributes according to "A.2.3 MEDCOM Header Module"* | | |
| Requesting Physician | (0032,1032) | From RIS |
| Requesting Service | (0032,1033) | From RIS |
| Requested Procedure Description | (0032,1060) | From RIS |
| Requested Procedure Code Sequence | (0032,1064) | From RIS |
| >Code Value | (0008,0100) | From RIS |
| >Coding Scheme Designator | (0008,0102) | From RIS |
| >Coding Scheme Version | (0008,0103) | From RIS |
| >Code Meaning | (0008,0104) | From RIS |
| Requested Contrast Agent | (0032,1070) | From RIS |
| Study Comments | (0032,4000) | "Exam Comment" input |
| Special Needs | (0038,0050) | From RIS |
| Patient State | (0038,0500) | From RIS |
| Performed Procedure Step Start Date | (0040,0244) | supplied, even if MPPS SOP class is not supported |
| Performed Procedure Step Start Time | (0040,0245) | supplied, even if MPPS SOP class is not supported |
| Performed Procedure Step ID | (0040,0253) | supplied, even if MPPS SOP class is not supported, "XAyyyymmddhhmmss" is set with 1st Image acquired |
| Request Attributes Sequence | (0040,0275) | only if SOP is done under Scheduled Procedure Step, else Sequence is not encoded |
| >Scheduled Procedure Step Description | (0040,0007) | From RIS |
| >Scheduled Procedure Step ID | (0040,0009) | From RIS |
| >Requested Procedure ID | (0040,1001) | From RIS or “Request ID” input |
| Confidentiality Constraint on Patient Data Description | (0040,3001) | From RIS |
| Curve Dimensions | (5000,0005) | 2 |
| Number of Points | (5000,0010) | <number of data points> |
| Type of Data | (5000,0020) | ECG |
| Axis Units | (5000,0030) | DPPS\NONE<br>(DPPS = data points per second) |
| Data Value Presentation | (5000,0103) | 0000h |
| Curve Data Descriptor | (5000,0110) | 0\1 |
| Coordinate Start Value | (5000,0112) | 0 |
| Coordinate Step Value | (5000,0114) | <sampling rate> |
| Curve Data | (5000,3000) | |
| Overlay Rows | (60xx,0010) | |
| Overlay Columns | (60xx,0011) | |
| Number of Frames in Overlay | (60xx,0015) | <number> |
| Overlay Description | (60xx,0022) | |
| Overlay Type | (60xx,0040) | G |
| Overlay Origin | (60xx,0050) | 1\1 |
| Image Frame Origin | (60xx,0051) | <1-based number> |
| Overlay Bits Allocated | (60xx,0100) | 1 or 16 (if uncompressed) |
| Overlay Bit Position | (60xx,0102) | 12 or 0 (if Overlay encoded in [60xx,3000]) |
| Overlay Data | (60xx,3000) | <contains Overlay> (not with uncompressed) |
| Pixel Data | (7FE0,0010) | |

Table 91 Overview of supplied attributes- X-Ray-Angiographic images (Original, Derived)

## A.5 Private Non-Image IOD

The Artis zee VC13 will create numerical data that cannot be correlated to an individual image instance and therefore need to be stored in separate instance(s). This is necessary to correlate the information in the right level of the DICOM data model hierarchy. Since there is no fitting DICOM SOP Class definition, SIEMENS has created a private “Non-Image IOD” to contain numerical data heaps to be managed within a DICOM structure. Please see previous chapters of the Appendix for IOD definition and the following tables for detailed encoding of the different “Non-Image SOP Class Instances”.

| Attribute Name | Tag | Value |
|---|---|---|
| Specific Character Set | (0008,0005) | from Configuration |
| Image Type | (0008,0008) | ORIGINAL\PRIMARY\SINGLE PLANE\\EXAM PROTOCOL |
| SOP Class UID | (0008,0016) | 1.3.12.2.1107.5.9.1 |
| SOP Instance UID | (0008,0018) | |
| Study Date | (0008,0020) | <yyyymmdd> |
| Series Date | (0008,0021) | <yyyymmdd> |
| Study Time | (0008,0030) | <hhmmss> |
| Series Time | (0008,0031) | <hhmmss> |
| Accession Number | (0008,0050) | RIS or “Accession Number” input |
| Modality | (0008,0060) | XA |
| Manufacturer | (0008,0070) | SIEMENS |
| Institution Name | (0008,0080) | |
| Referring Physician’s Name | (0008,0090) | RIS or input |
| Station Name | (0008,1010) | from Configuration |
| Study Description | (0008,1030) | “Study” input |
| Series Description | (0008,103E) | EXAM PROTOCOL |
| Performing Physician’s Name | (0008,1050) | input via “Correct” |
| Manufacturer’s Model Name | (0008,1090) | from Original |
| Patient’s Name | (0010,0010) | from Original |
| Patient ID | (0010,0020) | from Original |
| Patient’s Birth Date | (0010,0030) | from Original |
| Patient’s Sex | (0010,0040) | from Original |
| Patient’s Age | (0010,1010) | from Original |
| Device Serial Number | (0018,1000) | from Original |
| Software Version | (0018,1020) | from Original + “\<WS version>” |
| Study Instance UID | (0020,000D) | from Original |
| Series Instance UID | (0020,000E) | |
| Study ID | (0020,0010) | from Original |
| Series Number | (0020,0011) | |
| Image Number | (0020,0013) | |
| Patient Comments | (0020,4000) | "Exam Comment" input |
| Private Creator | (7FE1,00xx) | SIEMENS CSA NON-IMAGE |
| Non-Image Data | (7FE1,xx10) | <Exam Protocol data> (encoded as 8-Bit ASCII data, with <LF> as line separator) |

Table 92 Data Dictionary of private IOD Definition – Exam Protocol

## A.6 Quant Report Images

The Artis zee VC13 system will create result images from performing Quantitative Analysis Functions. To ensure image interchange, the resulting reports are converted to XA multi-frames with dedicated header data.

| Attribute Name | Tag | Value |
|---|---|---|
| Specific Character Set | (0008,0005) | From Configuration |
| Image Type | (0008,0008) | DERIVED\SECONDARY\<3rd to nth value from Original>\QUANT |
| SOP Class UID | (0008,0016) | 1.2.840.10008.5.1.4.1.1.12.1 |
| SOP Instance UID | (0008,0018) | |
| Study Date | (0008,0020) | <yyyymmdd> |
| Series Date | (0008,0021) | <yyyymmdd>(Quant Series) |
| Acquisition Date | (0008,0022) | Date of Original Acquisition |
| Content Date | (0008,0023) | <yyyymmdd> (Date of Creation) |
| Study Time | (0008,0030) | <hhmmss> |
| Series Time | (0008,0031) | <hhmmss> |
| Acquisition Time | (0008,0032) | Time of Original Acquisition |
| Content Time | (0008,0033) | <hhmmss> (Time of Creation) |
| Accession Number | (0008,0050) | From Original |
| Modality | (0008,0060) | XA |
| Manufacturer | (0008,0070) | Siemens |
| Institution Name | (0008,0080) | From Original |
| Referring Physician's Name | (0008,0090) | From Original |
| Station Name | (0008,1010) | from Configuration |
| Study Description | (0008,1030) | From Original |
| Series Description | (0008,103E) | Input from Analysis |
| Performing Physician's Name | (0008,1050) | From Original |
| Operator's Name | (0008,1070) | From Original |
| Admitting Diagnosis Description | (0008,1080) | From Original |
| Manufacturer's Model Name | (0008,1090) | AXIOM-Artis |
| Referenced Patient Sequence | (0008,1120) | From Original |
| >Referenced SOP Class UID | (0008,1150) | |
| >Referenced SOP Instance UID | (0008,1155) | |
| Start Trim | (0008,2142) | <1 st frame to display> |
| Stop Trim | (0008,2143) | <last frame to display> |
| Recomm. Display Frame Rate | (0008,2144) | (in f/s) |
| Patient's Name | (0010,0010) | From Original |
| Patient ID | (0010,0020) | From Original |
| Patient's Birth Date | (0010,0030) | From Original |
| Patient's Sex | (0010,0040) | From Original |
| Other Patient IDs | (0010,1000) | From Original |
| Other Patient Names | (0010,1001) | From Original |
| Patient's Age | (0010,1010) | From Original |
| Patient's Size | (0010,1020) | (in meters) |
| Patient‘s Weight | (0010,1030) | (in kilograms) |
| Medical Alerts | (0010,2000) | From Original |
| Contrast Allergies | (0010,2110) | From Original |
| Pregnancy Status | (0010,21C0) | From Original |
| Patient Comment | (0010,4000) | From Original |
| Contrast/Bolus Agent | (0018,0010) | From Original |

| Attribute Name | Tag | Value |
|---|---|---|
| Cine Rate | (0018,0040) | 1 |
| KVP | (0018,0060) | From Original |
| Device Serial Number | (0018,1000) | <modality serial number> |
| Software Version | (0018,1020) | |
| Protocol Name | (0018,1030) | From Original |
| Contrast Bolus Ingredient | (0018,1048) | From Original |
| Frame Time | (0018,1063) | 1000 |
| Distance Source to Detector | (0018,1110) | From Original |
| Distance Source to Patient | (0018,1111) | From Original |
| Exposure Time | (0018,1150) | <duration of x-Ray exposure>(msec) |
| X-Ray Tube Current | (0018,1151) | From Original |
| Average Pulse Width | (0018,1154) | From Original |
| Radiation Setting | (0018,1155) | From Original |
| Radiation Mode | (0018,115A) | From Original |
| Image and Fluoroscopy Area Dose Product | (0018,115E) | From Original |
| Intensifier Size | (0018,1162) | From Original |
| Imager Pixel Spacing | (0018,1164) | From Original |
| Focal Spot | (0018,1190) | From Original |
| Positioner Motion | (0018,1500) | From Original |
| Positioner Primary Angle | (0018,1510) | From Original |
| Positioner Secondary Angle | (0018,1511) | From Original |
| Positioner Primary Angle Increment | (0018,1520) | From Original (Only with DYNAMIC) |
| Positioner Secondary Angle Increment | (0018,1521) | From Original (Only with DYNAMIC) |
| Patient Position | (0018,5100) | From Original |
| Private Creator | (0019,00xx) | SIEMENS SMS-AX VIEW 1.0 |
| *Attributes according to "A.2.6 Angio Viewing Module"* | | |
| Study Instance UID | (0020,000D) | From Original |
| Series Instance UID | (0020,000E) | |
| Study ID | (0020,0010) | From Original |
| Series Number | (0020,0011) | |
| Acquisition Number | (0020,0012) | From Original |
| Instance Number | (0020,0013) | |
| Patient Orientation | (0020,0020) | From Original |
| Images in Acquisition | (0020,1002) | |
| Private Creator | (0021,00xx) | SIEMENS SMS-AX ACQ 1.0 |
| *Attributes according to "A.2.7 Angio Acquisition Data Module"* | | |
| Private Creator | (0023,00xx) | SIEMENS SMS-AX QUANT 1.0 |
| *Attributes according to "A.2.8 Angio Quantification Module" if image was calibrated* | | |
| Private Creator | (0025,00xx) | SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0 |
| *Attributes according to "A.2.9 Original Image Info Module"* | | |
| Samples per Pixel | (0028,0002) | 1 |
| Photometric Interpretation | (0028,0004) | MONOCHROME2 |
| Number of Frames | (0028,0008) | 1 to 4 |
| Frame Increment Pointer | (0028,0009) | (0018,1063) |
| Rows | (0028,0010) | 1024 |
| Columns | (0028,0011) | 1024 |
| Bits Allocated | (0028,0100) | 16 |
| Bits Stored | (0028,0101) | 12 |
| High Bit | (0028,0102) | 11 |
| Pixel Representation | (0028,0103) | 0 |
| Pixel Intensity Relationship | (0028,0103) | LIN |
| Window Center | (0028,1050) | 2047 |
| Window Width | (0028,1051) | 4095 |

| Attribute Name | Tag | Value |
|---|---|---|
| Lossy Image Compression | (0028,2110) | From Original |
| Representative Frame Number | (0028,6010) | 1 |
| Study Status ID | (0032,000A) | From Original |
| Scheduled Study Start Date | (0032,1000) | From Original |
| Scheduled Study Start Time | (0032,1001) | From Original |
| Scheduled Study Location | (0032,1020) | From Original |
| Scheduled Study Location AE Title(s) | (0032,1021) | From Original |
| Requesting Physician | (0032,1032) | From Original |
| Requesting Service | (0032,1033) | From Original |
| Requested Procedure Description | (0032,1060) | From Original |
| Requested Procedure Code Sequence | (0032,1064) | From Original |
| >Code Value | (0008,0100) | From Original |
| >Coding Scheme Designator | (0008,0102) | From Original |
| >Coding Scheme Version | (0008,0103) | From Original |
| >Code Meaning | (0008,0104) | From Original |
| Requested Contrast Agent | (0032,1070) | From Original |
| Study Comments | (0032,4000) | From Original |
| Performed Procedure Step Start Date | (0040,0244) | From Original |
| Performed Procedure Step Start Time | (0040,0245) | From Original |
| Performed Procedure Step ID | (0040,0253) | From Original |
| Request Attributes Sequence | (0040,0275) | From Original |
| >Scheduled Procedure Step Description | (0040,0007) | From Original |
| >Scheduled Procedure Step ID | (0040,0009) | From Original |
| >Requested Procedure ID | (0040,1001) | From Original |
| Confidentiality Constraint on Patient Data Description | (0040,3001) | From Original |
| Pixel Data | (7FE0,0010) | |

Table 93 Overview of supplied attributes- X-Ray-Angiographic image (Quant Report Image)

## A.7 CT/MR Image Converted to XA IOD

The Artis zee VC13 system will create reference images from CT or MR images. Those will be encoded as derived XA Standard Extended SOP Class. Please see the following table for a complete overview of supplied Type 1/2/3 Standard and additional Private Attributes:

| Attribute Name | Tag | Value |
|---|---|---|
| Specific Character Set | (0008,0005) | From Configuration |
| Image Type | (0008,0008) | See “A.2.10. SOP Common Module-Image Type Extensions” |
| SOP Class UID | (0008,0016) | 1.2.840.10008.5.1.4.1.1.12.1 |
| SOP Instance UID | (0008,0018) | <new UID> |
| Study Date | (0008,0020) | From Original or changed by CorRea (Drag & Drop) |
| Series Date | (0008,0021) | <yyyymmdd> |
| Acquisition Date | (0008,0022) | Date of Original Acquisition if provided by CT |
| Content Date | (0008,0023) | <yyyymmdd> (Date of Creation) |
| Study Time | (0008,0030) | From Original or changed by CorRea (Drag & Drop) |
| Series Time | (0008,0031) | <hhmmss> |
| Acquisition Time | (0008,0032) | Time of Original Acquisition |
| Content Time | (0008,0033) | <hhmmss> (Time of Creation) |
| Accession Number | (0008,0050) | From Original or changed by CorRea (Drag & Drop) |
| Modality | (0008,0060) | XA |
| Manufacturer | (0008,0070) | Siemens |
| Institution Name | (0008,0080) | From Original (Equipment) |
| Referring Physician's Name | (0008,0090) | From Original or changed by CorRea (Drag & Drop) |
| Station Name | (0008,1010) | Artis Station Name |
| Study Description | (0008,1030) | From Original or changed by CorRea (Drag & Drop) |
| Series Description | (0008,103E) | From Original |
| Institutional Department Name | (0008,1040) | From Original (Equipment) |
| Performing Physician's Name | (0008,1050) | From Original (series) |
| Operator's Name | (0008,1070) | From Original (series) |
| Admitting Diagnosis Description | (0008,1080) | From Original or changed by CorRea (Drag & Drop) |
| Manufacturer's Model Name | (0008,1090) | AXIOM-Artis |
| Source Image Sequence | (0008,2112) | Reference to original CT image |
| >Referenced SOP Class UID | (0008,1150) | 1.2.840.100008.5.1.4.1.1.2 (CT image) |
| >Referenced SOP Instance UID | (0008,1155) | From Original (0008,0018) |
| Patient‘s Name | (0010,0010) | From Original or changed by CorRea (Drag & Drop) |
| Patient ID | (0010,0020) | From Original or changed by CorRea (Drag & Drop) |
| Patient‘s Birth Date | (0010,0030) | From Original or changed by CorRea (Drag & Drop) |
| Patient‘s Sex | (0010,0040) | From Original or changed by CorRea (Drag & Drop) |
| Patient‘s Age | (0010,1010) | From Original or changed by CorRea (Drag & Drop) |
| Patient‘s Size | (0010,1020) | From Original or changed by CorRea (Drag & Drop) |
| Patient‘s Weight | (0010,1030) | From Original or changed by CorRea (Drag & Drop) |
| Medical Alerts | (0010,2000) | From Original |
| Contrast Allergies | (0010,2110) | From Original |
| Pregnancy Status | (0010,21C0) | From Original |
| Patient Comment | (0010,4000) | From Original or changed by CorRea (Drag & Drop) |
| Contrast/Bolus Agent | (0018,0010) | From Original (Contrast/Bolus) |
| KVP | (0018,0060) | From Original (image) |
| Device Serial Number | (0018,1000) | <Artis serial number> |
| Software Version | (0018,1020) | <Artis software version> |
| Protocol Name | (0018,1030) | From Original (Series Description) |

| Attribute Name | Tag | Value |
|---|---|---|
| Contrast Bolus Ingredient | (0018,1048) | From Original (Contrast/Bolus) |
| Estimated Radiographic Magnification Factor | (0018,1114) | 1.0 |
| Exposure Time | (0018,1150) | From Original (CT image) |
| X-Ray Tube Current | (0018,1151) | From Original (CT image) |
| Radiation Setting | (0018,1155) | GR |
| Image and Fluoroscopy Area Dose Product | (0018,115E) | <zero length> |
| Imager Pixel Spacing | (0018,1164) | Values taken from original "(0028,0030) Pixel Spacing" (Image Plane) |
| Positioner Primary Angle | (0018,1510) | <zero length> |
| Positioner Secondary Angle | (0018,1511) | <zero length> |
| Private Creator | (0019,00xx) | SIEMENS SMS-AX VIEW 1.0 |
| *Attributes according to "A.2.6 Angio Viewing Module"* | | |
| Study Instance UID | (0020,000D) | From Original or changed by CorRea (Drag & Drop) |
| Series Instance UID | (0020,000E) | <new UID> |
| Study ID | (0020,0010) | From Original or changed by CorRea (Drag & Drop) |
| Series Number | (0020,0011) | "1000-based counter" |
| Acquisition Number | (0020,0012) | From Original (image) |
| Instance Number | (0020,0013) | "2000-based" counter |
| Patient Orientation | (0020,0020) | From Original (series) |
| Images in Acquisition | (0020,1002) | |
| Image Comments | (0020,4000) | From Original (image) |
| Private Creator | (0021,00xx) | SIEMENS SMS-AX ACQ 1.0 |
| *Attributes according to "A.2.7 Angio Acquisition Data Module"* | | |
| Samples per Pixel | (0028,0002) | 1 |
| Photometric Interpretation | (0028,0004) | MONOCHROME2 |
| Rows | (0028,0010) | From Original (image) *only 512 supported* |
| Columns | (0028,0011) | From Original (image) *only 512 supported* |
| Bits Allocated | (0028,0100) | 16 |
| Bits Stored | (0028,0101) | 12 (converted) |
| High Bit | (0028,0102) | 11 (converted) |
| Pixel Representation | (0028,0103) | 0 (converted to unsigned) |
| Pixel Intensity Relationship | (0028,0103) | LIN or DISP |
| Window Center | (0028,1050) | Calculated from Original Window Center and Rescale intercept (VOI LUT, MOD LUT) |
| Window Width | (0028,1051) | From Original (VOI LUT) |
| Lossy Image Compression | (0028,2110) | From Original (image) |
| Study Status ID | (0032,000A) | From Original |
| Scheduled Study Start Date | (0032,1000) | From Original |
| Scheduled Study Start Time | (0032,1001) | From Original |
| Scheduled Study Location | (0032,1020) | From Original |
| Scheduled Study Location AE Title(s) | (0032,1021) | From Original |
| Requesting Physician | (0032,1032) | From Original |
| Requesting Service | (0032,1033) | From Original |
| Requested Procedure Description | (0032,1060) | From Original |
| Requested Contrast Agent | (0032,1070) | From Original |
| Study Comments | (0032,4000) | From Original or changed by CorRea (Drag & Drop) |
| Performed Procedure Step Start Date | (0040,0244) | From Original (series), if existent |
| Performed Procedure Step Start Time | (0040,0245) | From Original (series), if existent |
| Performed Procedure Step ID | (0040,0253) | From Original (series), if existent |
| Request Attributes Sequence | (0040,0275) | From Original (series), if existent |
| >item contents as provided | | As set from Original (series) |
| Overlay Rows | (60xx,0010) | Same as (0028,0010) |
| Overlay Columns | (60xx,0011) | Same as (0028,0011) |
| Overlay Description | (60xx,0022) | from Original (Overlay) |

| Attribute Name | Tag | Value |
|---|---|---|
| Overlay Type | (60xx,0040) | from Original (Overlay) |
| Overlay Origin | (60xx,0050) | 1\from Original (Overlay) |
| Overlay Bits Allocated | (60xx,0100) | from Original (Overlay) |
| Overlay Bit Position | (60xx,0102) | from Original (Overlay) |
| Overlay Data | [60xx,3000] | from Original (Overlay) |
| Pixel Data | (7FE0,0010) | Possibly converted from original pixel data |

Table 94 Overview of supplied attributes- XA image (Derived) from CT image

| Attribute Name | Tag | Value |
|---|---|---|
| Specific Character Set | (0008,0005) | From Configuration |
| Image Type | (0008,0008) | See “A.2.10. SOP Common Module-Image Type Extensions” |
| SOP Class UID | (0008,0016) | 1.2.840.10008.5.1.4.1.1.12.1 |
| SOP Instance UID | (0008,0018) | <new UID> |
| Study Date | (0008,0020) | From Original or changed by CorRea (Drag & Drop) |
| Series Date | (0008,0021) | <yyyymmdd> |
| Acquisition Date | (0008,0022) | Date of Original Acquisition if provided by MR |
| Content Date | (0008,0023) | <yyyymmdd> (Date of Creation) |
| Study Time | (0008,0030) | From Original or changed by CorRea (Drag & Drop) |
| Series Time | (0008,0031) | <hhmmss> |
| Acquisition Time | (0008,0032) | Time of Original Acquisition if provided by MR |
| Content Time | (0008,0033) | <hhmmss> (Time of Creation) |
| Accession Number | (0008,0050) | From Original or changed by CorRea (Drag & Drop) |
| Modality | (0008,0060) | XA |
| Manufacturer | (0008,0070) | Siemens |
| Institution Name | (0008,0080) | From Original (Equipment) |
| Referring Physician's Name | (0008,0090) | From Original or changed by CorRea (Drag & Drop) |
| Station Name | (0008,1010) | Artis Station Name |
| Study Description | (0008,1030) | From Original or changed by CorRea (Drag & Drop) |
| Series Description | (0008,103E) | From Original |
| Institutional Department Name | (0008,1040) | From Original (Equipment) |
| Performing Physician's Name | (0008,1050) | From Original (series) |
| Operator's Name | (0008,1070) | From Original (series) |
| Admitting Diagnosis Description | (0008,1080) | From Original or changed by CorRea (Drag & Drop) |
| Manufacturer's Model Name | (0008,1090) | AXIOM-Artis |
| Source Image Sequence | (0008,2112) | Reference to original MR image |
| >Referenced SOP Class UID | (0008,1150) | 1.2.840.100008.5.1.4.1.1.4 (MR image) |
| >Referenced SOP Instance UID | (0008,1155) | From Original (0008,0018) |
| Patient‘s Name | (0010,0010) | From Original or changed by CorRea (Drag & Drop) |
| Patient ID | (0010,0020) | From Original or changed by CorRea (Drag & Drop) |
| Patient‘s Birth Date | (0010,0030) | From Original or changed by CorRea (Drag & Drop) |
| Patient‘s Sex | (0010,0040) | From Original or changed by CorRea (Drag & Drop) |
| Patient‘s Age | (0010,1010) | From Original or changed by CorRea (Drag & Drop) |
| Patient‘s Size | (0010,1020) | From Original or changed by CorRea (Drag & Drop) |
| Patient‘s Weight | (0010,1030) | From Original or changed by CorRea (Drag & Drop) |
| Medical Alerts | (0010,2000) | From Original |
| Contrast Allergies | (0010,2110) | From Original |
| Pregnancy Status | (0010,21C0) | From Original |
| Patient Comment | (0010,4000) | From Original or changed by CorRea (Drag & Drop) |
| Contrast/Bolus Agent | (0018,0010) | From Original (Contrast/Bolus) |
| KVP | (0018,0060) | <zero length> |
| Device Serial Number | (0018,1000) | <Artis serial number> |

| Attribute Name | Tag | Value |
|---|---|---|
| Software Version | (0018,1020) | <Artis software version> |
| Protocol Name | (0018,1030) | From Original (Series Description) |
| Contrast Bolus Ingredient | (0018,1048) | From Original (Contrast/Bolus) |
| Estimated Radiographic Magnification Factor | (0018,1114) | 1.0 |
| Radiation Setting | (0018,1155) | SC (even if created w/o radiation!) |
| Image and Fluoroscopy Area Dose Product | (0018,115E) | <zero length> |
| Imager Pixel Spacing | (0018,1164) | Values taken from original "(0028,0030) Pixel Spacing" (Image Plane) |
| Positioner Primary Angle | (0018,1510) | <zero length> |
| Positioner Secondary Angle | (0018,1511) | <zero length> |
| Private Creator | (0019,00xx) | SIEMENS SMS-AX VIEW 1.0 |
| *Attributes according to "A.2.6 Angio Viewing Module"* | | |
| Study Instance UID | (0020,000D) | From Original or changed by CorRea (Drag & Drop) |
| Series Instance UID | (0020,000E) | <new UID> |
| Study ID | (0020,0010) | From Original or changed by CorRea (Drag & Drop) |
| Series Number | (0020,0011) | "1000-based counter" |
| Acquisition Number | (0020,0012) | From Original (image) |
| Instance Number | (0020,0013) | "2000-based" counter |
| Patient Orientation | (0020,0020) | From Original (series) |
| Images in Acquisition | (0020,1002) | |
| Image Comments | (0020,4000) | From Original (image) |
| Private Creator | (0021,00xx) | SIEMENS SMS-AX ACQ 1.0 |
| *Attributes according to "A.2.7 Angio Acquisition Data Module"* | | |
| Samples per Pixel | (0028,0002) | 1 |
| Photometric Interpretation | (0028,0004) | MONOCHROME2 |
| Rows | (0028,0010) | From Original (image) *only 512 supported* |
| Columns | (0028,0011) | From Original (image) *only 512 supported* |
| Bits Allocated | (0028,0100) | 16 |
| Bits Stored | (0028,0101) | 12 (converted) |
| High Bit | (0028,0102) | 11 (converted) |
| Pixel Representation | (0028,0103) | 0 (converted to unsigned) |
| Pixel Intensity Relationship | (0028,0103) | LIN or DISP |
| Window Center | (0028,1050) | Calculated from Original Window Center and Rescale intercept (VOI LUT, MOD LUT) |
| Window Width | (0028,1051) | From Original (VOI LUT) |
| Lossy Image Compression | (0028,2110) | From Original (image) |
| Study Status ID | (0032,000A) | From Original |
| Scheduled Study Start Date | (0032,1000) | From Original |
| Scheduled Study Start Time | (0032,1001) | From Original |
| Scheduled Study Location | (0032,1020) | From Original |
| Scheduled Study Location AE Title(s) | (0032,1021) | From Original |
| Requesting Physician | (0032,1032) | From Original |
| Requesting Service | (0032,1033) | From Original |
| Requested Procedure Description | (0032,1060) | From Original |
| Requested Contrast Agent | (0032,1070) | From Original |
| Study Comments | (0032,4000) | From Original or changed by CorRea (Drag & Drop) |
| Performed Procedure Step Start Date | (0040,0244) | From Original (series), if existent |
| Performed Procedure Step Start Time | (0040,0245) | From Original (series), if existent |
| Performed Procedure Step ID | (0040,0253) | From Original (series), if existent |
| Request Attributes Sequence | (0040,0275) | From Original (series), if existent |
| >item contents as provided | | As set from Original (series) |
| Overlay Rows | (60xx,0010) | Same as (0028,0010) |
| Overlay Columns | (60xx,0011) | Same as (0028,0011) |
| Overlay Description | (60xx,0022) | from Original (Overlay) |

| Attribute Name | Tag | Value |
|---|---|---|
| Overlay Type | (60xx,0040) | from Original (Overlay) |
| Overlay Origin | (60xx,0050) | 1\from Original (Overlay) |
| Overlay Bits Allocated | (60xx,0100) | from Original (Overlay) |
| Overlay Bit Position | (60xx,0102) | from Original (Overlay) |
| Overlay Data | [60xx,3000] | from Original (Overlay) |
| Pixel Data | (7FE0,0010) | Possibly converted from original pixel data |

Table 95 Overview of supplied attributes- XA image (Derived) from MR image

## A.8 Sorting Order Artis zee VC13

This section discusses the sorting algorithms for Artis within the patient browser and directory overview.

### A.8.1 Identification of Images

**Original acquired images** are identified by the following attribute contents:

| Attribute Name | Tag | Value |
|---|---|---|
| Image Type | (0008,0008) | ORIGINAL\PRIMARY\SINGLE PLANE\SINGLE A<br>ORIGINAL\PRIMARY\SINGLE PLANE\SINGLE B<br>ORIGINAL\PRIMARY\BIPLANE A<br>ORIGINAL\PRIMARY\BIPLANE B<br>ORIGINAL\PRIMARY\SINGLE PLANE\PLANE A\PERI\MASK\n<br>ORIGINAL\PRIMARY\SINGLE PLANE\PLANE A\PERI\FILL\n<br>ORIGINAL\PRIMARY\SINGLE PLANE\PLANE A\DYNA\MASK<br>ORIGINAL\PRIMARY\SINGLE PLANE\PLANE A\DYNA\INJECTION<br>ORIGINAL\PRIMARY\SINGLE PLANE\PLANE A\DYNA\FILL<br>ORIGINAL\PRIMARY\SINGLE PLANE\PLANE A\DYNA\WASHOUT<br>ORIGINAL\PRIMARY\SINGLE PLANE\SINGL A(B)\3D ACQ\DR<br>ORIGINAL\PRIMARY\SINGLE PLANE\SINGL A(B)\3D ACQ\DSA<br>ORIGINAL\PRIMARY\SINGLE PLANE\SINGL A(B)\3D ACQ\CARD<br>DERIVED\PRIMARY\SINGLE PLANE\SINGLE A\STORE FLUORO<br>DERIVED\PRIMARY\SINGLE PLANE\SINGLE B\STORE FLUORO<br>DERIVED\PRIMARY\BIPLANE A\\STORE FLUORO<br>DERIVED\PRIMARY\BIPLANE B\\STORE FLUORO |
| Series Time | (0008,0031) | Same as Acquisition Time |
| Acquisition Time | (0008,0032) | Time the acquisition of this image was performed |
| Content Time | (0008,0033) | Same as Acquisition Time (rule for acquired images) |
| Series Number | (0020,0011) | Same as Acquisition Number |
| Acquisition Number | (0020,0012) | Counts number of acquisitions. All images created during performance of this acquisition have the same number. |
| Instance Number | (0020,0013) | “1-based” counter for images. Indicates the creation order within the acquisition. |

Table 96 Identifications of images

**Store Monitor images,** derived from original images or Fluoro LIH, are identified by the following attribute contents:

| Attribute Name | Tag | Value |
|---|---|---|
| Image Type | (0008,0008) | DERIVED\SECONDARY\SINGLE PLANE\SINGLE A\STORE MONITOR<br>DERIVED\SECONDARY\SINGLE PLANE\SINGLE B\STORE MONITOR |
| Series Time | (0008,0031) | Same as Acquisition Time. Store Monitor is in same series. |
| Acquisition Time | (0008,0032) | Time the acquisition of the original image was performed |
| Content Time | (0008,0033) | Time this image was created (Store Monitor was performed) |
| Series Number | (0020,0011) | Same Number as Acquisition Number. (Reference to original Image) |
| Acquisition Number | (0020,0012) | Counts number of acquisitions. Refers to the acquisition number of the original image where this image was derived from. |
| Instance Number | (0020,0013) | "300-based" counter for images. Indicates the creation order of Store Monitor Reference images within this series |

Table 97 Identifications of Store Monitor images

**Store Reference images,** derived from original images or Fluoro LIH, are identified by the following attribute contents:

| Attribute Name | Tag | Value |
|---|---|---|
| Image Type | (0008,0008) | DERIVED\SECONDARY\SINGLE PLANE\SINGLE A\REFIMAGE<br>DERIVED\SECONDARY\SINGLE PLANE\SINGLE B\REFIMAGE |

| Attribute Name | Tag | Value |
|---|---|---|
| Series Time | (0008,0031) | Same as Acquisition Time. Store Reference image is in same series. |
| Acquisition Time | (0008,0032) | Time the acquisition of the original image was performed |
| Content Time | (0008,0033) | Time this image was created (Store Reference image was performed) |
| Series Number | (0020,0011) | Same Number as Acquisition Number. (Reference to original Image) |
| Acquisition Number | (0020,0012) | Counts number of acquisitions. Refers to the acquisition number of the original image where this image was derived from. |
| Instance Number | (0020,0013) | "100-based" counter for images. Indicates the creation order of Store Reference images within this series |

Table 98 Identifications of Reference images

**Quant Report images,** derived from original images or Fluoro LIH, are identified by the following attribute contents:

| Attribute Name | Tag | Value |
|---|---|---|
| Image Type | (0008,0008) | DERIVED\SECONDARY\SINGLE PLANE\SINGLE A\QUANT<br>DERIVED\SECONDARY\SINGLE PLANE\SINGLE B\QUANT |
| Series Time | (0008,0031) | Time this Quant image was created (Quant was performed) |
| Acquisition Time | (0008,0032) | Time the acquisition of the original image was performed |
| Content Time | (0008,0033) | Time this Quant image was created (Quant was performed) |
| Series Number | (0020,0011) | Same Number as Acquisition Number. (Reference to original Image) |
| Acquisition Number | (0020,0012) | Counts number of acquisitions. Refers to the acquisition number of the original image where this image was derived from. |
| Instance Number | (0020,0013) | "1-based" counter for images. Quant Reports are stored in new series. |

Table 99 Identifications of Quant report images

**EXAM PROTOCOL non-image,** created once per study, is identified by the following attribute contents:

| Attribute Name | Tag | Value |
|---|---|---|
| Image Type | (0008,0008) | ORIGINAL\PRIMARY\SINGLE PLANE\\EXAM PROTOCOL |
| SOP Class UID | (0008,0016) | 1.3.12.2.1107.5.9.1 |
| Series Time | (0008,0031) | Exam Protocol is allocated with Patient Registration. |
| Acquisition Time | (0008,0032) | Not set |
| Content Time | (0008,0033) | Not set |
| Series Number | (0020,0011) | Fixed value of "999" |
| Acquisition Number | (0020,0012) | Not set |
| Instance Number | (0020,0013) | Not set |

Table 100 Identifications of Exam Protocol non-images

**EXAM PROTOCOL as XA image,** created during transfer of EXAM PROTOCOL non-image, is identified by the following attribute contents:

| Attribute Name | Tag | Value |
|---|---|---|
| Image Type | (0008,0008) | ORIGINAL\PRIMARY\SINGLE PLANE\SINGLE A\EXAM PROTOCOL |
| SOP Class UID | (0008,0016) | 1.2.840.10008.5.1.4.1.1.12.1 |
| Series Time | (0008,0031) | Exam Protocol is allocated with Patient Registration. |
| Acquisition Time | (0008,0032) | Time this protocol was created (i.e. transferred) |
| Content Time | (0008,0033) | Time this protocol was created (i.e. transferred) |
| Series Number | (0020,0011) | Fixed value of "999" |
| Acquisition Number | (0020,0012) | Fixed value of "999" |
| Instance Number | (0020,0013) | Fixed value of "999" |

Table 101 Identifications of Exam Protocol as XA image

### A.8.2 The Sorting Algorithms of the Artis Viewer

Artis zee VC13 has implemented sorting algorithms to display DICOM objects in the directory overview in a specific order. Sorting/Grouping in the Viewer Directory Overview occurs according the following rules:

1. Sort by Series Number

2. If Series Number matches: Group on Series Number, Sort by Instance Number

3. If Series Number and Instance Number each match: Group on Series Number, Sort by Content Time

In the case, that the user has selected "Scenes + Ref Images" or "Scenes + Store Monitor", the reference images or the store monitor images follow directly the image they had been derived from.

**Example 1:**

Patient "Test 1" with one Study, three Series with one acquired image, three Store Monitor Images and one Reference Image in each Series. "Scenes" is selected under the "Dir Overview" button => only the acquired images are displayed.

**Patient “Test 1”**

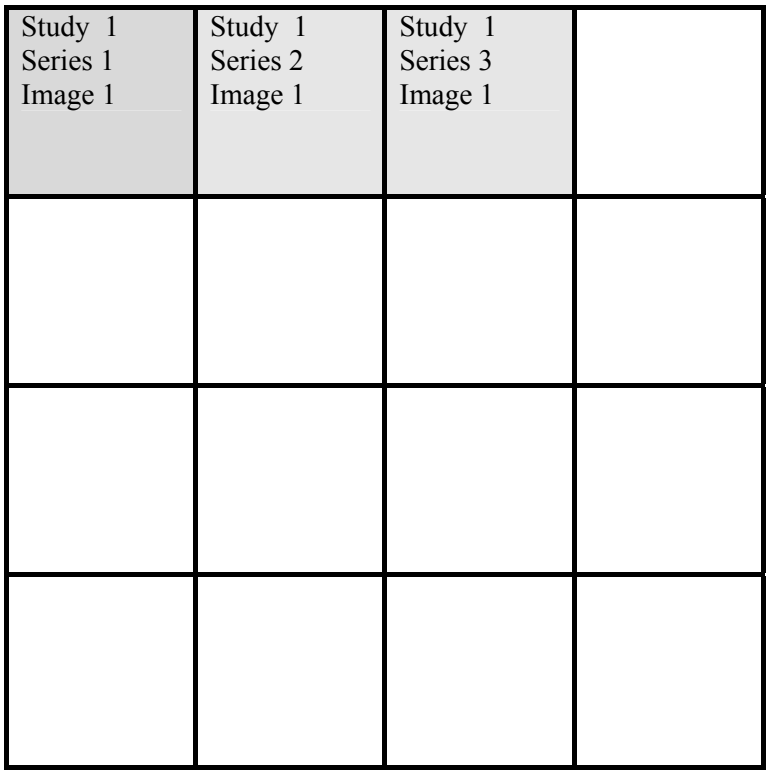


Figure 11 Image ordering – simple case

**Example 2:**

Patient "Test 2" with one Study, three Series with one acquired image, three Store Monitor Images and one Reference Image in each Series. "Scenes + Ref Images" is selected under the "Dir Overview" button => the acquired images and the corresponding reference images are displayed.

**Patient "Test 2"**

| | | | |
|---|---|---|---|
| Study 1<br>Series 1<br>Image 1 | Study 1<br>Series 1<br>Image 100 | Study 1<br>Series 2<br>Image 1 | Study 1<br>Series 2<br>Image 100 |
| Study 1<br>Series 3<br>Image 1 | Study 1<br>Series 3<br>Image 100 | | |
| | | | |
| | | | |

| | |
|---|---|
| | Acquired Image |
| | Store Monitor Image |
| | Store Reference Image |

Figure 12 Image ordering – with Reference images

**Example 3:**

Patient "Test 3" with one Study, three Series with one acquired image, three Store Monitor Images and one Reference Image in each Series. "Scenes + Store Monitor" is selected under the "Dir Overview" button => the acquired images and the corresponding store monitor images are displayed.

**Patient "Test 31"**

| | | | |
|---|---|---|---|
| Study 1<br>Series 1<br>Image 1 | Study 1<br>Series 1<br>Image 300 | Study 1<br>Series 1<br>Image 301 | Study 1<br>Series 1<br>Image 302 |
| Study 1<br>Series 2<br>Image 1 | Study 1<br>Series 2<br>Image 300 | Study 1<br>Series 2<br>Image 301 | Study 1<br>Series 2<br>Image 302 |
| Study 1<br>Series 3<br>Image 1 | Study 1<br>Series 3<br>Image 300 | Study 1<br>Series 3<br>Image 301 | Study 1<br>Series 3<br>Image 302 |
| | | | |

| | |
|---|---|
| | Acquired Image |
| | Store Monitor Image |
| | Store Reference Image |

Figure 13 Image ordering – with Store Monitor images

**Example 4:**

For Scene #2 of Patient "Test 3" now a Quant Report is performed. According to Example 3, the Overview now sorts as follows:

**Patient "Test 1"**

| | | | |
|---|---|---|---|
| Study 1<br>Series 1<br>Image 1 | Study 1<br>Series 1<br>Image 300 | Study 1<br>Series 1<br>Image 301 | Study 1<br>Series 1<br>Image 302 |
| Study 1<br>Series 2<br>Image 1 | Study 1<br>Series 2(Quant)<br>Image 1(Quant) | Study 1<br>Series 2<br>Image 300 | Study 1<br>Series 2<br>Image 301 |
| Study 1<br>Series 2<br>Image 302 | Study 1<br>Series 3<br>Image 300 | Study 1<br>Series 3<br>Image 301 | Study 1<br>Series 3<br>Image 302 |
| Study 1<br>Series 3<br>Image 1 | | | |

| | |
|---|---|
| | Acquired Image |
| | Store Monitor Image |
| | Store Reference Image |
| | Quant Report Image |

Figure 14 Image ordering – with Store Monitor and Quant images

### A.8.3 The Sorting Algorithms of Artis Browser

Besides the default sorting criteria, Artis supports the following sorting algorithms for the patient browser.

The default syngo sorting settings are as follows

- Artis displays images - within a Series - with the order they had been acquired

- Artis displays Series - within a Study - with the order they had been acquired

- Artis displays Studies - within a Patient - with the order they had been acquired

Therefore the Quant Report Series will not necessarily be displayed adjacent to the original scene, if created later at the end of all scenes.

## A.9 Supported Matrix Sizes of Artis zee VC13

Depending on detector size and mode the Artis zee VC13 supports different matrix sizes. These matrix sizes are also used by the Storage AE when sending the images to a remote SCP. Additionally it is possible to send images resized to 512x512 and 1024x1024 (see also 5.1.2.1.6).

Artis zee VC13 uses following original Matrix Sizes:

| Detector Size | Rows (0028,0010) | Columns (0028,0011) |
|---|---|---|
| FD 30x40 | 2480 | 1920 |
| | 1920 | 2480 |
| | 1920 | 1920 |
| | 1440 | 1440 |
| | 1240 | 960 |
| | 1024 | 1024 |
| | 960 | 1240 |
| | 960 | 960 |
| | 720 | 720 |
| | 616 | 480 |
| | 512 | 512 |
| | 480 | 616 |
| | 480 | 480 |
| | 360 | 360 |
| | 256 | 256 |
| FD 20x20 | 960 | 960 |
| | 776 | 776 |
| | 600 | 600 |
| | 480 | 480 |
| | 384 | 384 |
| | 296 | 296 |
| | 192 | 192 |

Table 102 Supported Matrix Sizes

## A.10 DICOM Print SCU – detailed status displays

The following tables document the behavior of the Artis zee VC13 DICOM Print AE in response to messages received for the printer SOP class and the print job SOP class.

Definitions of camera symbols:

- Idle: Camera is installed and ready; idle icon is displayed.
- Interact: The user has to react in near future, but not immediately.
  Example: A camera was low in 8x10 clear sheets: LOW 8x10 CLR was sent by n-event-report.
- Queue Stopped: The user has to react immediately. Either the camera needs immediate interaction or a job has been aborted.
  Example: A camera is out of 8x10 clear sheets, or camera is down, or a film job is aborted.

Note: different camera symbols are displayed according to the Printer Status Info.

The Printer Status (Success, Warning, Failure) is not evaluated, since the Printer Status Info is much more detailed and allows a more appropriate reaction of the system.

### A.10.1 Common Status Information

*"Printer Status Infos within Printer SOP Class/Execution Status Infos within Print Job SOP class"*

| Printer Status Info/ Execution Status Info | Description | Message string visible in 'Status Bar' | Other action for UI/ 'camera symbol' |
|---|---|---|---|
| NORMAL | Camera is ready | Camera is ready | <None>/idle |
| BAD RECEIVE MGZ | There is a problem with the film receive magazine. Films from the printer cannot be transported into the magazine. | Problem with receive magazine. | <None>/interact |
| BAD SUPPLY MGZ | There is a problem with the film supply magazine. Films from this magazine cannot be transported into the printer. | Problem with supply magazine. | <None>/interact |
| CALIBRATING | Printer is performing self calibration, it is expected to be available for normal operation shortly. | Self calibration. Please wait. | <None>/idle |
| CALIBRATION ERR | An error in the printer calibration has been detected, quality of processed films may not be optimal. | Problem in calibration. Film quality may not be optimal. | <None>/interact |
| CHECK CHEMISTRY | A problem with the processor chemicals has been detected, quality of processed films may not be optimal. | Problem with chemistry. Film quality may not be optimal. | <None>/interact |
| CHECK SORTER | There is an error in the film sorter | Error in film sorter. | <None>/interact |
| CHEMICALS EMPTY | There are no processing chemicals in the processor, films will not be printed and processed until the processor is back to normal. | Camera chemistry empty. Please check. | <None>/interact |
| CHEMICALS LOW | The chemical level in the processor is low, if not corrected, it will probably shut down soon. | Camera chemistry low. Please check. | <None>/interact |
| COVER OPEN | One or more printer or processor covers, drawers, doors are open. | Camera cover, drawer or door open. | <None>/interact |
| ELEC CONFIG ERR | Printer configured improperly for this job. | Camera configured improperly for this job. Queue stopped. | **Queue for this camera will be STOPPED/ Queue stopped** |

| Printer Status Info/ Execution Status Info | Description | Message string visible in 'Status Bar' | Other action for UI/ 'camera symbol' |
|---|---|---|---|
| ELEC DOWN | Printer is not operating due to some unspecified electrical hardware problem. | Camera electrical hardware Problem. | <None>/interact |
| ELEC SW ERROR | Printer not operating for some unspecified software error. | Camera software problem. Queue stopped. | **Queue for this camera will be STOPPED/ Queue stopped** |
| EMPTY 8x10 | The 8x10 inch film supply magazine is empty. | 8x10 film supply empty. | <None>/interact |
| EMPTY 8x10 BLUE | The 8x10 inch blue film supply magazine is empty. | 8x10 blue film supply empty. | <None>/interact |
| EMPTY 8x10 CLR | The 8x10 inch clear film supply magazine is empty. | 8x10 clear film supply empty. | <None>/interact |
| EMPTY 8x10 PAPR | The 8x10 inch paper supply magazine is empty. | 8x10 paper supply empty. | <None>/interact |
| EMPTY 10x12 | The 10x12 inch film supply magazine is empty. | 10x12 film supply empty. | <None>/interact |
| EMPTY 10x12 BLUE | The 10x12 inch blue film supply magazine is empty. | 10x12 blue film supply empty. | <None>/interact |
| EMPTY 10x12 CLR | The 10x12 inch clear film supply magazine is empty. | 10x12 clear film supply empty. | <None>/interact |
| EMPTY 10x12 PAPR | The 10x12 inch paper supply magazine is empty. | 10x12 paper supply empty. | <None>/interact |
| EMPTY 10x14 | The 10x14 inch film supply magazine is empty. | 10x14 film supply empty. | <None>/interact |
| EMPTY 10x14 BLUE | The 10x14 inch blue film supply magazine is empty. | 10x14 blue film supply empty. | <None>/interact |
| EMPTY 10x14 CLR | The 10x14 inch clear film supply magazine is empty. | 10x14 clear film supply empty. | <None>/interact |
| EMPTY 10x14 PAPR | The 10x14 inch paper supply magazine is empty. | 10x14 paper supply empty. | <None>/interact |
| EMPTY 11x14 | The 11x14 inch film supply magazine is empty. | 11x14 film supply empty. | <None>/interact |
| EMPTY 11x14 BLUE | The 11x14 inch blue film supply magazine is empty. | 11x14 blue film supply empty. | <None>/interact |
| EMPTY 11x14 CLR | The 11x14 inch clear film supply magazine is empty. | 11x14 clear film supply empty. | <None>/interact |
| EMPTY 11x14 PAPR | The 11x14 inch paper supply magazine is empty. | 11x14 paper supply empty. | <None>/interact |
| EMPTY 14x14 | The 14x14 inch film supply magazine is empty. | 14x14 film supply empty. | <None>/interact |
| EMPTY 14x14 BLUE | The 14x14 inch blue film supply magazine is empty. | 14x14 blue film supply empty. | <None>/interact |
| EMPTY 14x14 CLR | The 14x14 inch clear film supply magazine is empty. | 14x14 clear film supply empty. | <None>/interact |
| EMPTY 14x14 PAPR | The 14x14 inch paper supply magazine is empty. | 14x14 paper supply empty. | <None>/interact |
| EMPTY 14x17 | The 14x17 inch film supply magazine is empty. | 14x17 film supply empty. | <None>/interact |
| EMPTY 14x17 BLUE | The 14x17 inch blue film supply magazine is empty. | 14x17 blue film supply empty. | <None>/interact |
| EMPTY 14x17 CLR | The 14x17 inch clear film supply magazine is empty. | 14x17 clear film supply empty. | <None>/interact |
| EMPTY 14x17 PAPR | The 14x17 inch paper supply magazine is empty. | 14x17 paper supply empty. | <None>/interact |
| EMPTY 24x24 | The 24x24 inch film supply magazine is empty. | 24x24 film supply empty. | <None>/interact |
| EMPTY 24x24 BLUE | The 24x24 inch blue film supply magazine is empty. | 24x24 blue film supply empty. | <None>/interact |
| EMPTY 24x24 CLR | The 24x24 inch clear film supply magazine is empty. | 24x24 clear film supply empty. | <None>/interact |
| EMPTY 24x24 PAPR | The 24x24 inch paper supply magazine is empty. | 24x24 paper supply empty | <None>/interact |
| EMPTY 24x30 | The 24x30 inch film supply magazine is empty. | 24x30 film supply empty. | <None>/interact |
| EMPTY 24x30 BLUE | The 24x30 inch blue film supply magazine is empty. | 24x30 blue film supply empty. | <None>/interact |
| EMPTY 24x30 CLR | The 24x30 inch clear film supply magazine is empty. | 24x30 clear film supply empty. | <None>/interact |

| Printer Status Info/ Execution Status Info | Description | Message string visible in 'Status Bar' | Other action for UI/ 'camera symbol' |
|---|---|---|---|
| EMPTY 24x30 PAPR | The 24x30 inch paper supply magazine is empty. | 24x30 paper supply empty. | <None>/interact |
| EMPTY A4 PAPR | The A4 paper supply magazine is empty. | A4 paper supply empty | <None>/interact |
| EMPTY A4 TRANS | The A4 transparency supply magazine is empty. | A4 transparency supply empty. | <None>/interact |
| EXPOSURE FAILURE | The exposure device has failed due to some unspecified reason. | Exposure device has failed. | <None>/interact |
| FILM JAM | A film transport error has occurred and a film is jammed in the printer or processor. | Film jam. | <None>/interact |
| FILM TRANSP ERR | There is a malfunction with the film transport, there may or may not be a film jam. | Film transport problem. | <None>/interact |
| FINISHER EMPTY | The finisher is empty. | Finisher is empty. | <None>/interact |
| FINISHER ERROR | The finisher is not operating due to some unspecified reason | Finisher problem. | <None>/interact |
| FINISHER LOW | The finisher is low on supplies. | Finisher low. | <None>/interact |
| LOW 8x10 | The 8x10 inch film supply magazine is low. | 8x10 film supply low. | <None>/interact |
| LOW 8x10 BLUE | The 8x10 inch blue film supply magazine is low. | 8x10 blue film supply low. | <None>/interact |
| LOW 8x10 CLR | The 8x10 inch clear film supply magazine is low. | 8x10 clear film supply low. | <None>/interact |
| LOW 8x10 PAPR | The 8x10 inch paper supply magazine is low. | 8x10 paper supply low. | <None>/interact |
| LOW 10x12 | The 10x12 inch film supply magazine is low. | 10x12 film supply low. | <None>/interact |
| LOW 10x12 BLUE | The 10x12 inch blue film supply magazine is low. | 10x12 blue film supply low. | <None>/interact |
| LOW 10x12 CLR | The 10x12 inch clear film supply magazine is low. | 10x12 clear film supply low. | <None>/interact |
| LOW 10x12 PAPR | The 10x12 inch paper supply magazine is low. | 10x12 paper supply low. | <None>/interact |
| LOW 10x14 | The 10x14 inch film supply magazine is low. | 10x14 film supply low. | <None>/interact |
| LOW 10x14 BLUE | The 10x14 inch blue film supply magazine is low. | 10x14 blue film supply low. | <None>/interact |
| LOW 10x14 CLR | The 10x14 inch clear film supply magazine is low. | 10x14 clear film supply low. | <None>/interact |
| LOW 10x14 PAPR | The 10x14 inch paper supply magazine is low. | 10x14 paper supply low. | <None>/interact |
| LOW 11x14 | The 11x14 inch film supply magazine is low. | 11x14 film supply low. | <None>/interact |
| LOW 11x14 BLUE | The 11x14 inch blue film supply magazine is low. | 11x14 blue film supply low. | <None>/interact |
| LOW 11x14 CLR | The 11x14 inch clear film supply magazine is low. | 11x14 clear film supply low. | <None>/interact |
| LOW 11x14 PAPR | The 11x14 inch paper supply magazine is low. | 11x14 paper supply low. | <None>/interact |
| LOW 14x14 | The 14x14 inch film supply magazine is low. | 14x14 film supply low. | <None>/interact |
| LOW 14x14 BLUE | The 14x14 inch blue film supply magazine is low. | 14x14 blue film supply low. | <None>/interact |
| LOW 14x14 CLR | The 14x14 inch clear film supply magazine is low. | 14x14 clear film supply low. | <None>/interact |
| LOW 14x14 PAPR | The 14x14 inch paper supply magazine is low. | 14x14 paper supply low. | <None>/interact |
| LOW 14x17 | The 14x17 inch film supply magazine is low. | 14x17 film supply low. | <None>/interact |
| LOW 14x17 BLUE | The 14x17 inch blue film supply magazine is low. | 14x17 blue film supply low. | <None>/interact |
| LOW 14x17 CLR | The 14x17 inch clear film supply magazine is low. | 14x17 clear film supply low. | <None>/interact |
| LOW 14x17 PAPR | The 14x17 inch paper supply magazine is low. | 14x17 paper supply low. | <None>/interact |
| LOW 24x24 | The 24x24 inch film supply magazine is low. | 24x24 film supply low. | <None>/interact |

| Printer Status Info/ Execution Status Info | Description | Message string visible in 'Status Bar' | Other action for UI/ 'camera symbol' |
|---|---|---|---|
| LOW 24x24 BLUE | The 24x24 inch blue film supply magazine is low. | 24x24 blue film supply low. | <None>/interact |
| LOW 24x24 CLR | The 24x24 inch clear film supply magazine is low. | 24x24 clear film supply low. | <None>/interact |
| LOW 24x24 PAPR | The 24x24 inch paper supply magazine is low. | 24x24 paper supply low. | <None>/interact |
| LOW 24x30 | The 24x30 inch film supply magazine is low. | 24x30 film supply low. | <None>/interact |
| LOW 24x30 BLUE | The 24x30 inch blue film supply magazine is low. | 24x30 blue film supply low. | <None>/interact |
| LOW 24x30 CLR | The 24x30 inch clear film supply magazine is low. | 24x30 clear film supply low. | <None>/interact |
| LOW 24x30 PAPR | The 24x30 inch paper supply magazine is low. | 24x30 paper supply low. | <None>/interact |
| LOW A4 PAPR | The A4 paper supply magazine is low. | A4 paper supply low. | <None>/interact |
| LOW A4 TRANS | The A4 transparency supply magazine is low.. | A4 transparency supply low. | <None>/interact |
| NO RECEIVE MGZ | The film receive magazine is not available. | Film receiver not available. | <None>/interact |
| NO RIBBON | The ribbon cartridge needs to be replaced. | Replace ribbon cartridge. | <None>/interact |
| NO SUPPLY MGZ | The film supply magazine specified for this job is not available. | Film supply not available. | <None>/interact |
| CHECK PRINTER | The printer is not ready at this time, operator intervention is required to make the printer available. | Check camera. | <None>/interact |
| CHECK PROC | The processor is not ready at this time, operator intervention is required to make the printer available. | Check processor. | <None>/interact |
| PRINTER DOWN | The printer is not operating due to some unspecified reason. | Camera down. | <None>/interact |
| PRINTER INIT | The printer is not ready at this time, it is expected to become available without intervention. For example, it may be in a normal warm-up state. | Camera initializing. | <None>/Idle |
| PRINTER OFFLINE | The printer has been disabled by an operator or service person. | Camera off-line. | <None>/interact |
| PROC DOWN | The processor is not operating due to some unspecified reason. | Processor down. | <None>/interact |
| PROC INIT | The processor is not ready at this time, it is expected to become available without intervention. For example, it may be in a normal warm-up state. | Processor initializing. | <None>/Idle |
| PROC OVERFLOW FL | Processor chemicals are approaching the overflow full mark. | Processor chemicals near overflow. | <None>/interact |
| PROC OVERFLOW HI | Processor chemicals have reached the overflow full mark. | Processor chemicals overflow. | <None>/interact |
| QUEUED | Print job in Queue | -- | <None>/Idle |
| RECEIVER FULL | The film receive magazine is full. | Receiver full. | <None>/interact |
| REQ MED NOT INST | The requested film, paper, or other media supply magazine is installed in the printer, but may be available with operator intervention. | Install media supply. | <None>/interact |
| REQ MED NOT AVAI | The requested film, paper, or other media requested is not available on this printer. | Media supply not available on this camera. Queue stopped. Change camera. | **Queue for this camera will be STOPPED/ Queue stopped** |
| RIBBON ERROR | There is an unspecified problem with the print ribbon. | Error with print ribbon. | <None>/interact |
| SUPPLY EMPTY | The printer is out of film. | Camera out of film. | <None>/interact |
| SUPPLY LOW | The film supply is low. | Film supply low. | <None>/interact |
| UNKNOWN | There is an unspecified problem. | Unspecified problem with camera. | <None>/interact |

Table 103 Printer Status Information

### A.10.2 Additional Status Information – AGFA printers

*"Printer Status Infos: Additional Agfa printer Status Infos"*

| Printer Status Info/ Execution Status Info | Description | Message string visible in 'Status Bar' | Other action for UI/ 'camera symbol' |
|---|---|---|---|
| WARMING UP | Printer is in the warm-up stage. Spooling of print jobs to disk is still possible. | Camera is warming up. | <None>/idle |
| OFFLINE | OFFLINE Printer is switched off-line. Spooling of print jobs to disk is still possible. | Camera is switched off-line. | <None>/interact |
| NONE | General printer warning, no specific information is available. Spooling of print jobs to disk is still possible. | -- | <None>/idle |

Table 104 Printer Status Information - Agfa

### A.10.3 Additional Status Information – Kodak PACS Link (formerly Imation)

*"Printer Status Infos: Additional Kodak infos for PACS Link (formerly Imation Cameras)"*

| Printer Status Info/ Execution Status Info | Description | Message string visible in 'Status Bar' | Other action for UI/ 'camera symbol' |
|---|---|---|---|
| SUPPLY MGZ ERR | The supply magazine has an error. | Film supply has an error. | <None>/interact |

Table 105 Printer Status Information – Kodak (Imation)

### A.10.4 Additional Status Information – Kodak 190

*"Printer Status Infos: Additional Kodak infos for Kodak 190"*

| Printer Status Info/ Execution Status Info | Description | Message string visible in 'Status Bar' | Other action for UI/ 'camera symbol' |
|---|---|---|---|
| PRINTER STOPPED | The printer has stopped. | Camera has stopped. | <None>/interact |
| FATAL ERROR | Fatal Error. | Fatal Error. Queue stopped. | **Queue for this camera will be STOPPED/ Queue stopped** |

Table 106 Printer Status Information – Kodak 190

## A.10.5 Additional Status Information – Kodak 2180/1120

*"Printer Status Infos: Additional Kodak infos for Kodak 2180/1120"*

| Printer Status Info/ Execution Status Info | Description | Message string visible in 'Status Bar' | Other action for UI/ 'camera symbol' |
|---|---|---|---|
| PRINTER NOT RDY | Printer not ready. | Camera not ready.. | <None>/interact |
| CHECK PROCESSOR | Check processor. | Check processor. | <None>/interact |
| NO TONER | No toner. | No toner. | <None>/interact |
| FATAL | Fatal Error. | Fatal Error. Queue stopped. | **Queue for this camera will be STOPPED/ Queue stopped** |

Table 107 Printer Status Information – Kodak 2180/1120

## A.10.6 Additional Status Information – Codonics

| Printer Status Info/ Execution Status Info | Description | Message string visible in 'Status Bar' | Other action for UI/ 'camera symbol' |
|---|---|---|---|
| STANDARD | Printer is ready. | Camera is ready. | <None>/Normal |
| LOAD A-SIZE | Load A-Size media. | Load A-Size media. | <None>/interact |
| LOAD A-DVPAPER | Load A-Size black and white paper. | Load A-Size black and white paper. | <None>/interact |
| LOAD A-CVPAPER | Load A-Size color paper. | Load A-Size color paper. | <None>/interact |
| LOAD A-CVTRANS | Load A-Size transparencies. | Load A-Size transparencies. | <None>/interact |
| LOAD A4-SIZE | Load A4-Size media. | Load A4-Size media. | <None>/interact |
| LOAD A4-DVPAPER | Load A4-Size black and white paper. | Load A4-Size black and white paper. | <None>/interact |
| LOAD A4-CVPAPER | Load A4-Size color paper. | Load A4-Size color paper. | <None>/interact |
| LOAD A4-CVTRANS | Load A4-Size transparencies. | Load A4-Size transparencies. | <None>/interact |
| LOAD LA-SIZE | Load LA-Size media. | Load LA-Size media. | <None>/interact |
| LOAD LA-DVPAPER | Load LA-Size black and white paper. | Load LA-Size black and white paper. | <None>/interact |
| LOAD LA-CVPAPER | Load LA-Size color paper. | Load LA-Size color paper. | <None>/interact |
| LOAD LA-CVTRANS | Load LA-Size transparencies. | Load LA-Size transparencies. | <None>/interact |
| LOAD LA4-SIZE | Load LA4-Size media. | Load LA4-Size media. | <None>/interact |
| LOAD LA4-DVPAPER | Load LA4-Size black and white paper. | Load LA4-Size black and white paper. | <None>/interact |
| LOAD LA4-CVPAPER | Load LA4-Size color paper. | Load LA4-Size color paper. | <None>/interact |
| LOAD LA4-CVTRANS | Load LA4-Size transparencies. | Load LA4-Size transparencies. | <None>/interact |
| LOAD XLA-SIZE | Load XLA-Size media. | Load XLA-Size media. | <None>/interact |
| LOAD XLA-DVPAPER | Load XLA-Size black and white paper. | Load XLA-Size black and white paper. | <None>/interact |
| LOAD XLA-CVPAPER | Load XLA-Size color paper. | Load XLA-Size color paper. | <None>/interact |
| LOAD XLA-CVTRANS | Load XLA-Size transparencies. | Load XLA-Size transparencies. | <None>/interact |
| LOAD XLA4-SIZE | Load XLA4-Size media. | Load XLA4-Size media. | <None>/interact |
| LOAD XLA4-DVPAPER | Load XLA4-Size black and white paper. | Load XLA4-Size black and white paper. | <None>/interact |
| LOAD XLA4-CVPAPER | Load XLA4-Size color paper. | Load XLA4-Size color paper. | <None>/interact |
| LOAD XLA4-CVTRANS | Load XLA4-Size transparencies. | Load XLA4-Size transparencies. | <None>/interact |
| LOAD XLW-SIZE | Load XLW-Size media. | Load XLW-Size media. | <None>/interact |
| LOAD XLW-DVPAPER | Load XLW-Size black and white paper. | Load XLW-Size black and white paper. | <None>/interact |

| Printer Status Info/ Execution Status Info | Description | Message string visible in 'Status Bar' | Other action for UI/ 'camera symbol' |
|---|---|---|---|
| LOAD XLW-CVPAPER | Load XLW-Size color paper. | Load XLW-Size color paper. | <None>/interact |
| LOAD 8X10-SIZE | Load 8x10 media. | Load 8x10 media. | <None>/interact |
| LOAD 8X10-DVFILM | Load XLW-Size black and white film. | Load XLW-Size black and white film. | <None>/interact |
| SUPPLY MISSING | The film supply magazine specified for this job is not available. | Film supply not available. | <None>/interact |
| RIBBON MISSING | Ribbon is missing. | Ribbon is missing. | <None>/interact |
| RIBBON EMPTY | Ribbon is empty. | Ribbon is empty. | <None>/interact |
| TOP COVER OPEN | Top cover of printer is open. | Top cover of camera is open. | <None>/interact |

Table 108 Printer Status Information – Codonics

## A.10.7 Additional DICOM Execution Status Information

| Printer Status Info/ Execution Status Info | Description | Message string visible in 'Status Bar' | Other action for UI/ 'camera symbol' |
|---|---|---|---|
| INVALID PAGE DES | The specified page layout cannot be printed or other page description errors have been detected. | Film Job cannot be printed on this camera. Queue stopped. Please redirect film job. | **Queue for this camera will be STOPPED/ Queue stopped** |
| INSUFFICIENT MEMORY | There is not enough memory available to complete this job. | Not enough memory available in camera. Queue stopped. Please continue queue or change camera. | **Queue for this camera will be STOPPED/ Queue stopped** |
| NONE | General printer warning, no specific information is available. Spooling of print jobs to disk is still possible. | -- | <None>/Idle |

Table 109 Additional DICOM Execution Status Infos